

A detailed 3D rendering of a dental implant. It features a long, tapered, metallic abutment with a hexagonal top, which is being inserted into a multi-layered, cylindrical implant body. The implant body has a textured, porous appearance. The background is a light gray with abstract blue and white geometric lines.

Ufit[®] dental implant

The Ufit[®] Dental Implant History.

2001 JULY	Established T.STRONG (Manufacturer) Reported One year Clinical Experiments
2002 MAY	Registered Product Licensed by the Korea Food & Drug Administration (KFDA). Brand Name: UFIT Registered Product Licensed by the Busan Regional Korea Food & Drug Administration
2003 SEP	Recognition of Materials & Components Enterprise by MCT (Materials & Components Technology) Certified ANSI/ISO/ASQ Q9001-2000. Certificate NO: 17162-QMS-2538 Contracted for Dental Implant Technical in cooperation with KIMM (KOREA INSTITUTE OF MACHINERY AND MATERIAL)
2003 OCT	Applied Patent Registration for Torque Wrench Driver Adapter
2004 FEB	Applied Patent Registration for Dental Locking Abutment
2004 FEB	Established T.STRONG INC. (Corporation)
2004 MAR	Acquired Patent Registration for Torque Wrench Driver Adapter (Registration No. 0345598)
2004 MAY	Acquired Patent Registration for Dental Locking Abutment (Registration No. 0350606)
2004 AUG	Participated in Gyeong Nam Regional Specialized Industry and Technology Development (GYEONGNAM REGIONAL INNOVATION AGENCY, KOREA INSTITUTE OF SCIENCE AND TECHNOLOGY EVALUATION AND PLANNING)
2004 SEP	Contracted for Dental Implant Technology in cooperation with KIMM (KOREA INSTITUTE OF MACHINERY & MATERIAL)
2004 OCT	Signed an Agreement for Technology Development for the Removal of 3D (Difficulty, Dirty, Danger) in Manufacturing (KOREA INSTITUTE OF INDUSTRIAL TECHNOLOGY) Success of TRANSPLANTATION test for External and Internal Type Dental Implant System (KOREA TESTING AND RESEARCH INSTITUTE)
2004 NOV	Designated as a CLEAN place of business (Ministry of Labor)
2004 DEC	Received a Commendation for Medical and Pharmaceutical Product superiority and Good Example Enterprise

2005 JUN	Signed an Agreement for Technology Development (CHANGWON UNIVERSITY)
2005 OCT	Acquired Product License (Grade:4) from the KOREA FOOD AND DRUG ADMINISTRATION (KFDA)
2006 APR	Selected as Top Company with Best Technology Innovation in Business and Brand Sector by Sports Seoul
2007 SEP	Acquired Certification from KOREA GOOD MANUFACTURING PRACTICE (KGMP) (Certificate No.: MGK-537)
2008 JAN	SYLBUTMENT Development
2009 SEP	SYLBUTMENT Application

2010 FEB	Applied Domestic Patent for SYLBUTMENT
2010 JUN	Registered Product License of SYLBUTMENT and Launching
2010 JUL	Registered Product License of Hybrid Surface Treatment of Laser Neck Implant
2010 NOV	Renewal of KGMP Certificate (Certificate NO: KTR-AB-090778)
2011 FEB	Applied PCT Patent for SYLBUTMENT
2011 JUL	Received Certified ISO 13485 License, CE Product License (GT2 Fixture)

2012 JAN	Received Domestic Patent for SYLBUTMENT (Certificate NO:10-1109625)
2012 MAR	Registration of the trademark
	Attend PHARMED & HEALTHCARE VIETNAM
2012 DEC	Received Certified ISO 13485, ISO 9001 License, and CE Product License (SGS, Notified Body 0120)


2013 JUL	Received Japan Patent for SYLBUTMENT (Patent NO: 5291256)
	Renewal of KGMP Certificate (Certificate NO: KCL-ABB-130007)
2013 SEP	Participate Moscow Dental Expo 2013 Moscow
2013 OCT	Turkey Visit, DMA Dilman, Exclusive Distributor
	Participate World Dental Show(WDS) 2013 Mumbai

2014 FEB	Participate AEEDC Dubai 2014 UAE
2014 JUN	Received U.S FDA Certificate (Certificate NO: K132956)
	Rouyesh Novin Med-Iran Exclusive Distributor, Meeting In Korea
2014 DEC	Participate Greater New York Dental Meeting(GNYDM) 2014 New York

2015 JAN	Implamarket-Kazakhstan Exclusive Distributor, Meeting In Korea
2015 FEB	Received China Patent for Sylbutment (Patent NO: ZL 2011 8 0005727.3)
2015 MAR	Participate International Dental Show(IDS) 2015 German
2015 SEP	Abutment Quality Guarantee Enforcement
	Participate FDI Annual Dental Congress 2015 Bangkok
2015 DEC	Received Certified ISO 13485, ISO 9001 License, and CE Product License (SGS, Notified Body 0120)

2016 FEB	Participate AEEDC Dubai 2016
2016 JUL	Renewal of KGMP Certificate (Certificate NO: KCL-ABB-160009)

Dental implant Fixture & Abutment

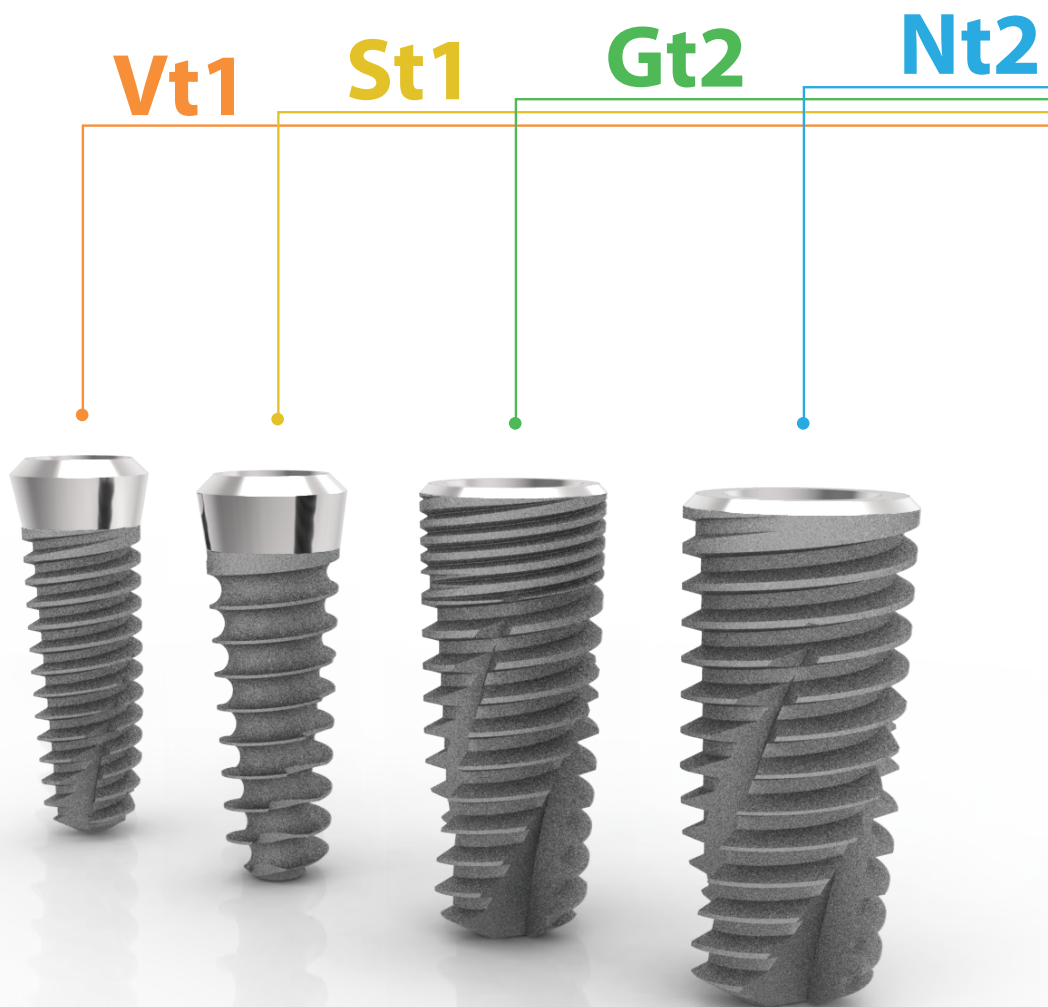

A revolution in dental implant systems

SYLBUTMENT is the product of engineering research in which the perfect contact of two flat surfaces is only possible theoretically but practically impossible.



Unprecedented - a remarkable sealing effect

The Sealing Effect occurs because of elastic modification done by the pressure on the circular bands of the contact sides.



Outstanding durability due to even stress distribution

The even contact surfaces uniformly transfer power from prosthetic appliances to fixtures. Results of fatigue tests showed that not a single fatigue failure occurred when repeated high stress loads were applied.



NO Gap

The circular bands act as a cushion within the limits of elastic modification when chewing force is applied.



NO Loosening

The even surface contact of the circular grooved pattern evenly distributes chewing force within the limits of elasticity, preventing the screw from loosening and the abutment from swaying.

The principles of SYLBUTMENT™

The principles of SYLBUTMENT are easily discovered around us.



Tire treads




Sealing effect of a piston ring




Soles of shoes

Conventional Abutment and SYLBUTMENT™

In a conventional abutment, the gap between fixture and abutment may increase gradually due to repeated chewing forces. This is due to the contact between the outer surface of the abutment and the inner taper of the fixture, which only occurs on a small surface area due to the roughness of both the two surfaces. On the other hand, SYLBUTMENT increases the contact surfaces by transformation to the grooves. It does not create a gap as the transformation between the two surfaces occurs within the elastic range.

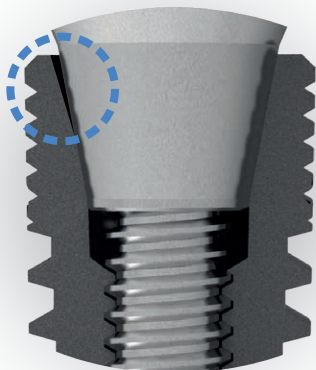


Conventional Abutment

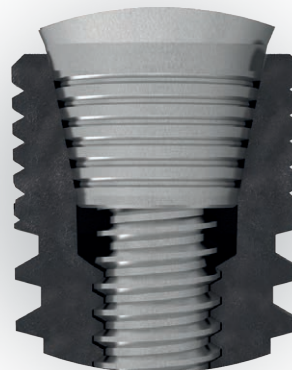

SYLBUTMENT™


Why does loosening occur in conventional abutments?

The perfect contact of two flat surfaces is only possible theoretically but practically impossible.

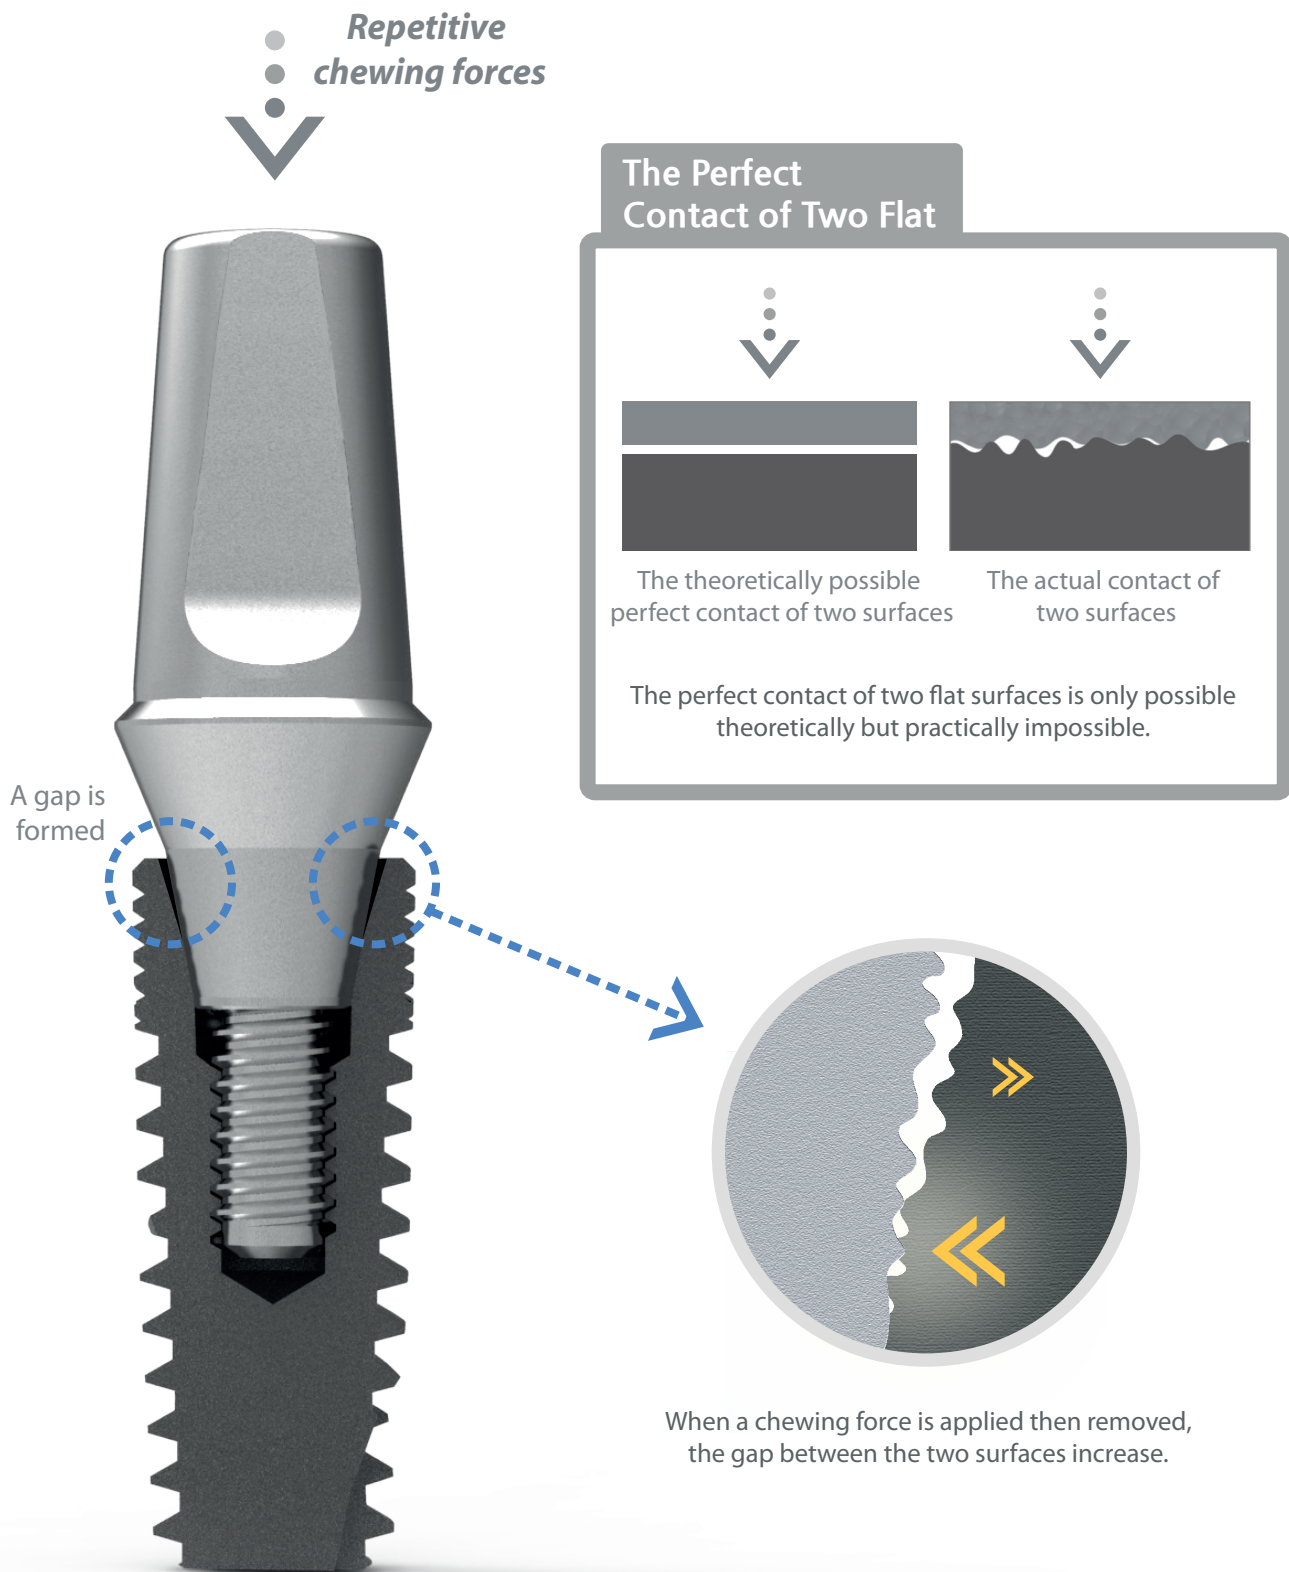


The reason why SYLBUTMENT™ is strong against fatigue (1)

When the abutment screw is fastened, elastic deformation occurs around the grooves of the SYLBUTMENT, creating a force which moves the abutment and fixture together.

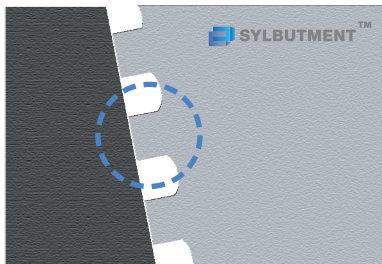


*Before fastening
the Abutment Screw*

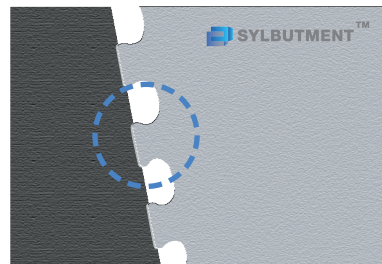

*After fastening
the Abutment Screw*


The reason why SYLBUTMENT™ is strong against fatigue (2)

As shown in the figure above, chewing forces are experienced asymmetrically due to the grooves of the SYLBUTMENT acting as an elastic body. This firmly maintains the sealed state of the abutment and distributes the chewing forces evenly in the fixture.

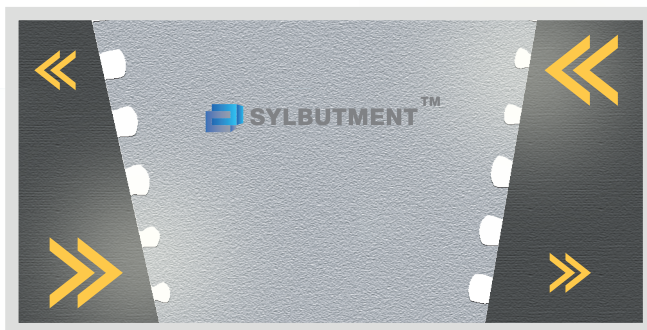


*The circular pattern section of
SYLBUTMENT™ receiving chewing forces*

SYLBUTMENT™

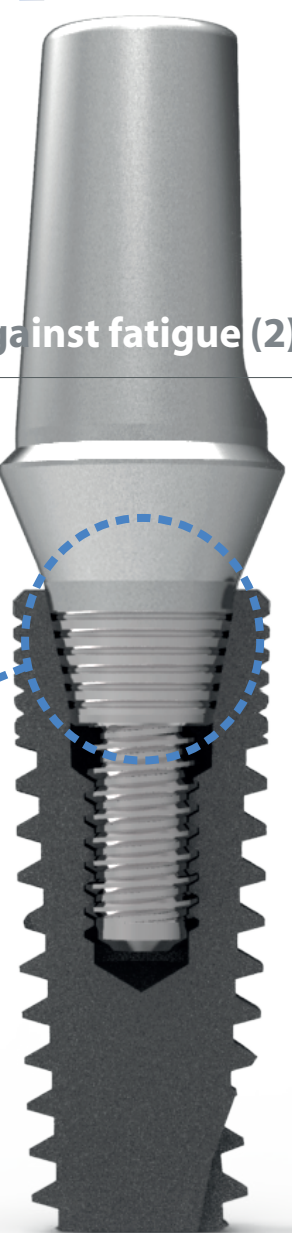


Pressure distribution at the contact surfaces of the Fixtures and the Abutments (FEM Analysis)

When conventional abutments experience asymmetrical chewing forces, the contact surfaces of the fixtures and abutments are separated; however, when a SYLBUTMENT is used, the contact surfaces are not separated.

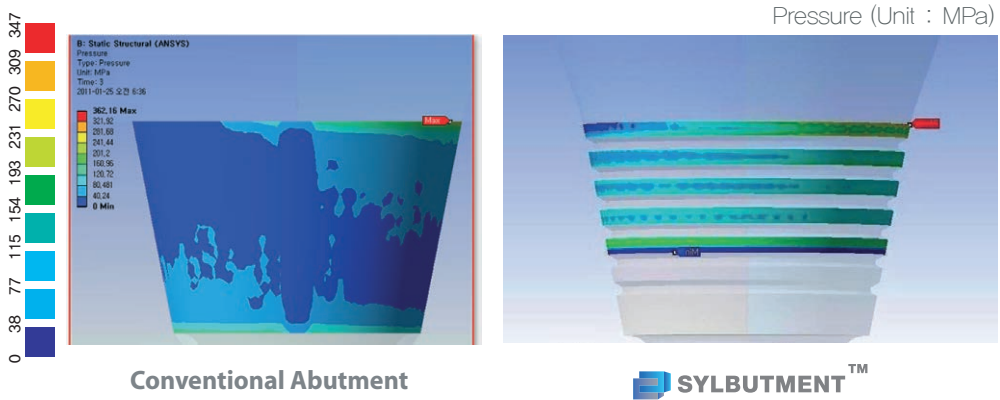

Fatigue tests of the SYLBUTMENT™

Conventional Abutments can withstand 5 million repeated loads of 344N~34N, but the SYLBUTMENT can withstand 5 million repeated loads of 552N~55N.

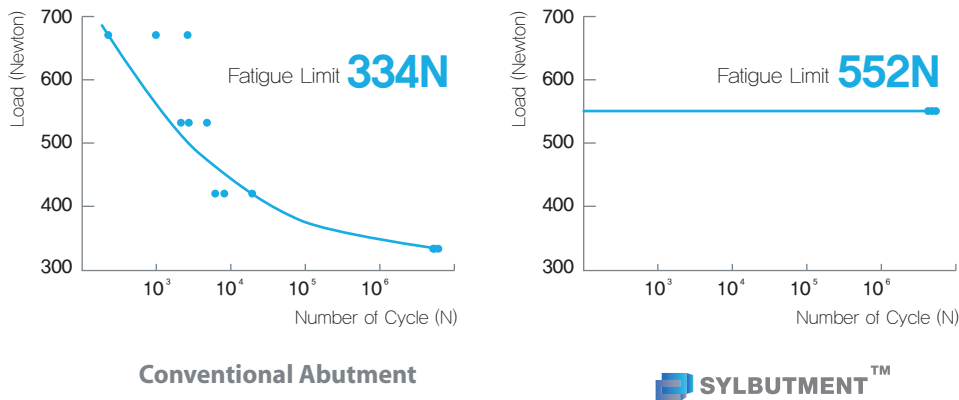


Submerged Fixture

Gt2

Connection


2.5 Hex indentation and 11 degree Morse Taper.



Micro Thread


The deep 0.2 mm micro thread increases the surface area and induces a smooth connection with the larger main thread. Additionally, the micro thread increases thread contact with bone thereby improving the initial fixation effect.

Dual Thread



As 0.8mm pitch of dual thread type, the surgery time is reduced. (1.6mm per 1 rotation)

RBM Surface



Surface areas are increased through blasting by highly biocompatible Calcium-Phosphate Media.

Main Thread

When the fixture is inserted into the implant bed, the conical shape and lower deep thread of the fixture increase stability and make immediate loading possible.


Cutting Edge



When placing the implants, the cutting edge of the Twist Type increases Self Tapping ability and minimizes Bone resistance.

Apex


Apex has the dimension of $D(\text{fixture diameter}) - 0.7\text{mm}$ and the body shape has the overall tapered one.

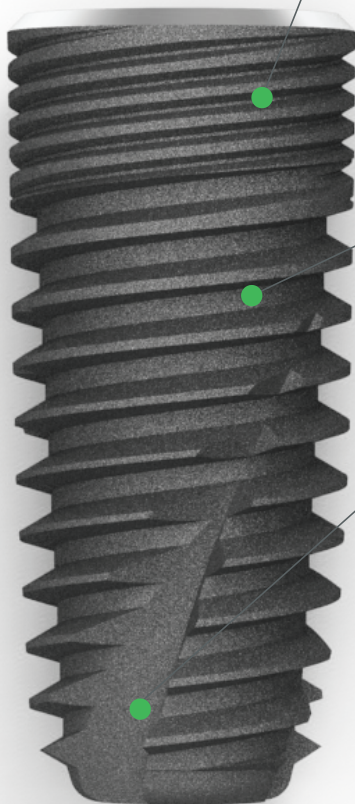


Nt2

Connection

2.5 Hex fastening Type of 11 degree Morse Taper Type




Dual Thread




As 0.8 Dual Thread Type, the placing speed is very fast. (1.6mm per 1 rotation)

RBM Surface



Surface areas are increased through blasting by highly biocompatible Calcium-Phosphate Media.

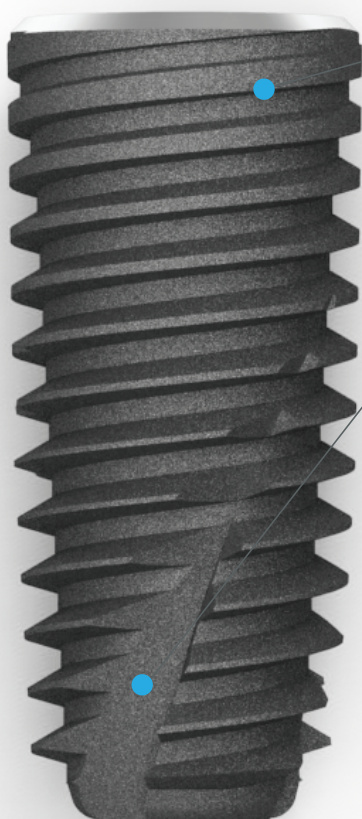


Main Thread

When the fixture is inserted into the implant bed, the conical shape and lower deep thread of the fixture increase stability and make immediate loading possible.

Cutting Edge




When placing the implants, the cutting edge of the Twist Type increases Self Tapping ability and minimizes Bone resistance.




Apex


As a structure of D (Diameter) - 0.7mm, the overall Tapered type

Submerged system Flow chart

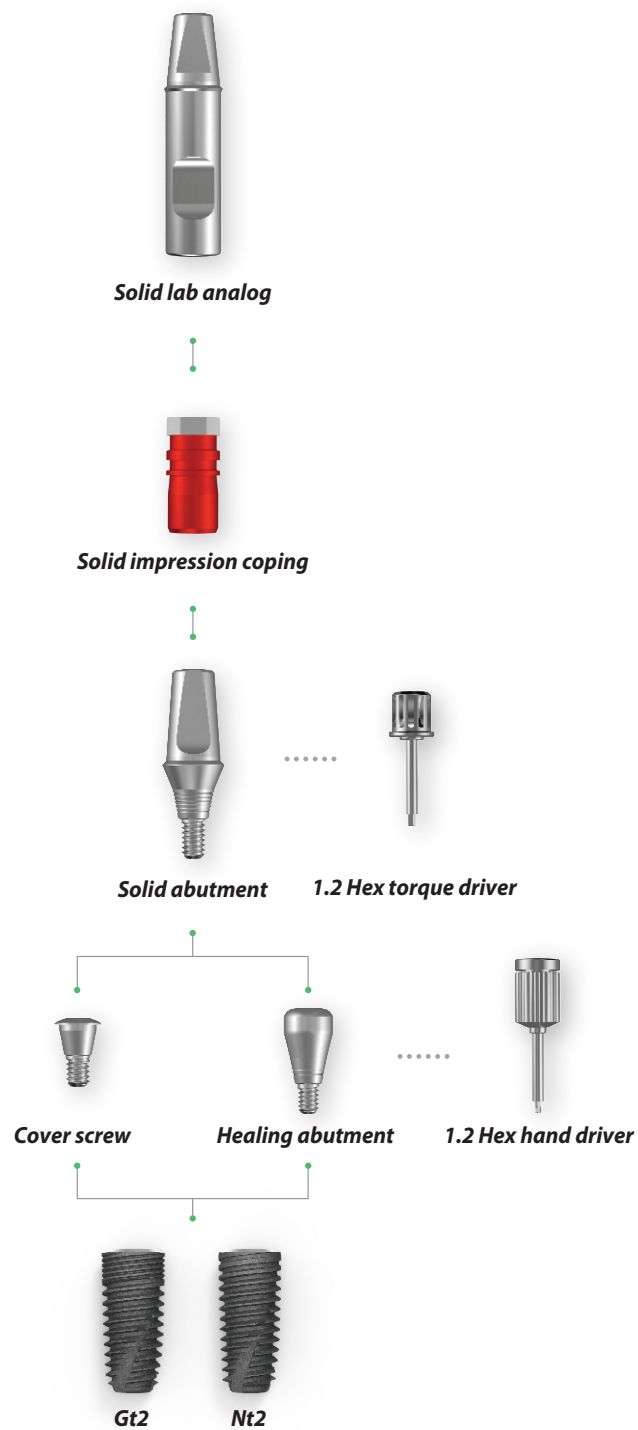

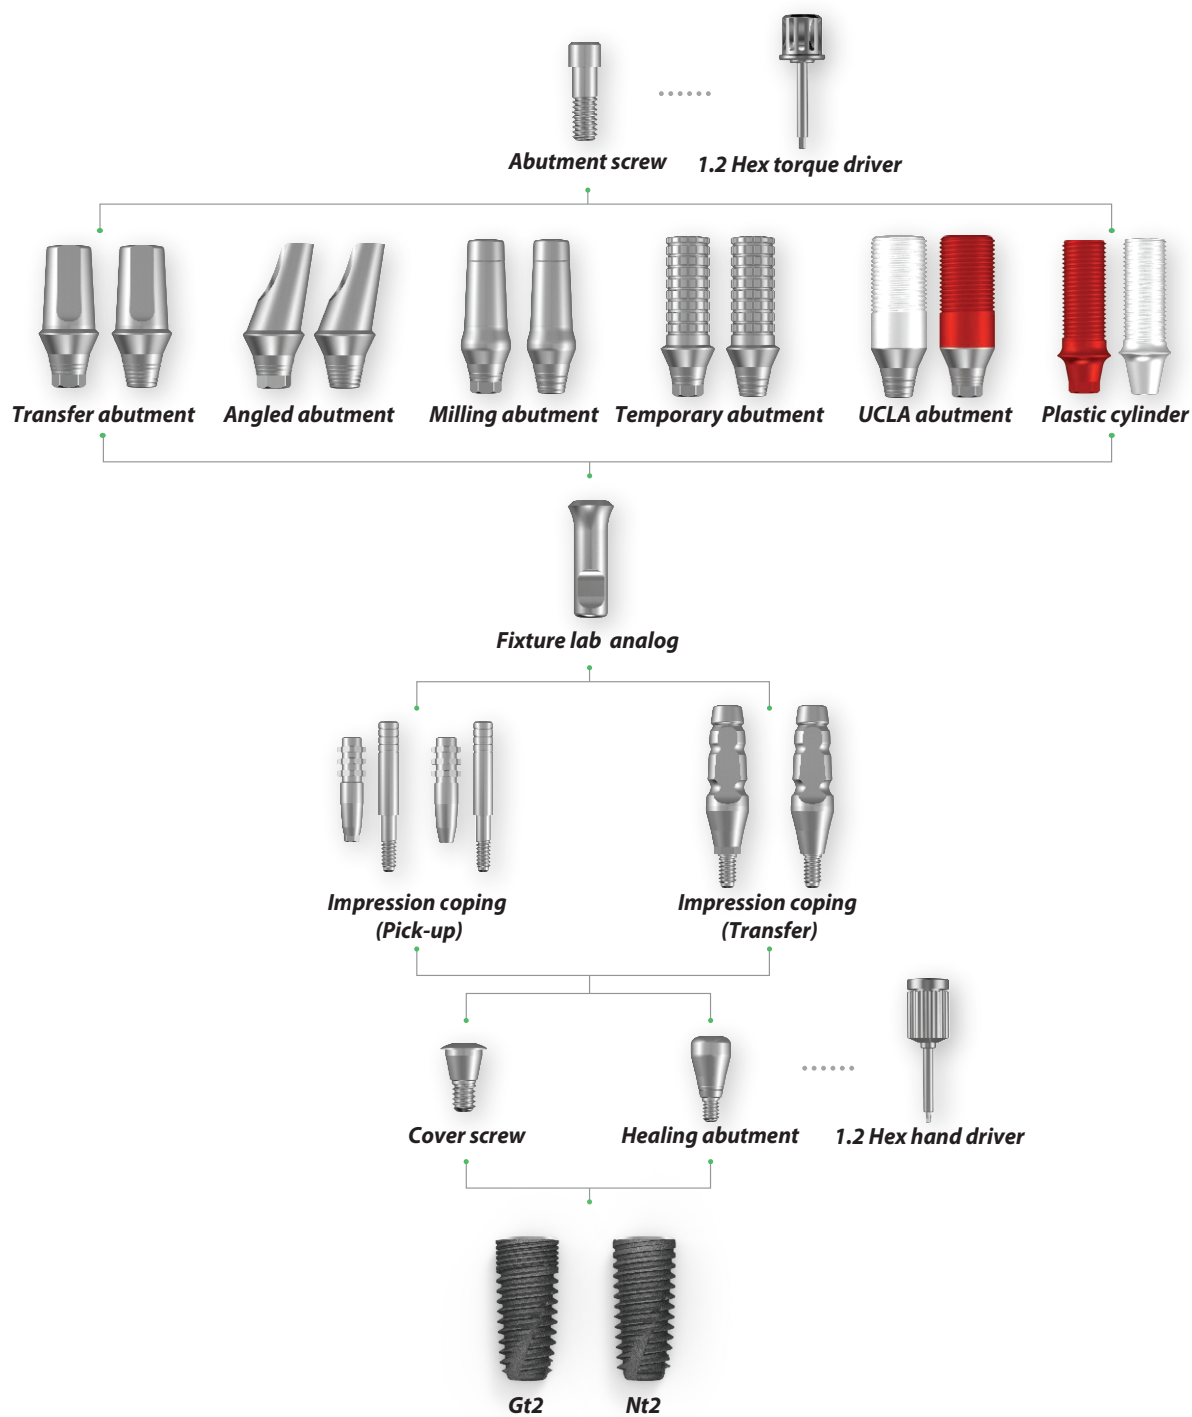

Submerged Fixture

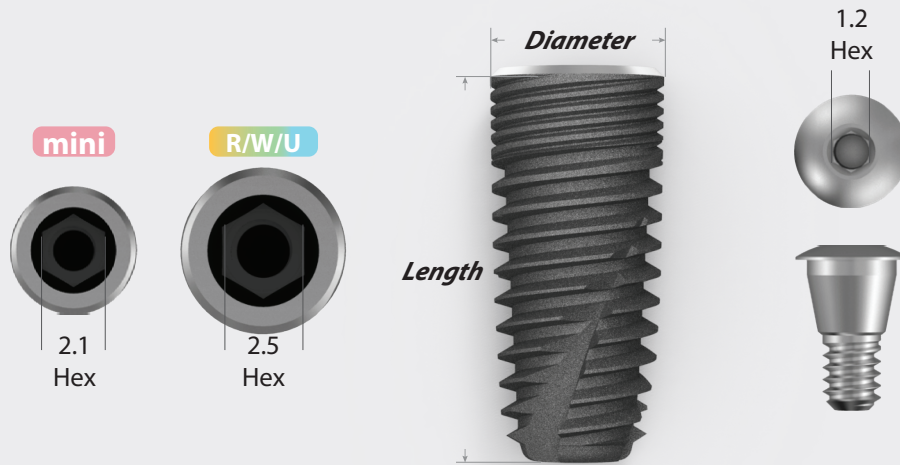

Gt2 mini

Length ● **D3.5**

8.5	GT2 35085 MT
10	GT2 3510 MT
11.5	GT2 35115 MT
13	GT2 3513 MT

* Use mini size abutment


- Mini
- Regular
- Wide
- Ultra-wide

Gt2 R/W/U

Length	● D4.0	● D4.5	● D5.0
7	GT2 4007 MT	GT2 4507 MT	GT2 5007 MT
8.5	GT2 40085 MT	GT2 45085 MT	GT2 50085 MT
10	GT2 4010 MT	GT2 4510 MT	GT2 5010 MT
11.5	GT2 40115 MT	GT2 45115 MT	GT2 50115 MT
13	GT2 4013 MT	GT2 4513 MT	GT2 5013 MT

Length	● D5.5	● D6.0	● D6.5	● D7.0
7	GT2 5507 MT	GT2 6007 MT	GT2 6507 MT	GT2 7007 MT
8.5	GT2 55085 MT	GT2 60085 MT	GT2 65085 MT	GT2 70085 MT
10	GT2 5510 MT	GT2 6010 MT	GT2 6510 MT	GT2 7010 MT
11.5	GT2 55115 MT	GT2 60115 MT	GT2 65115 MT	GT2 70115 MT
13	GT2 5513 MT	GT2 6013 MT	GT2 6513 MT	GT2 7013 MT

* Use R/W/U size abutment

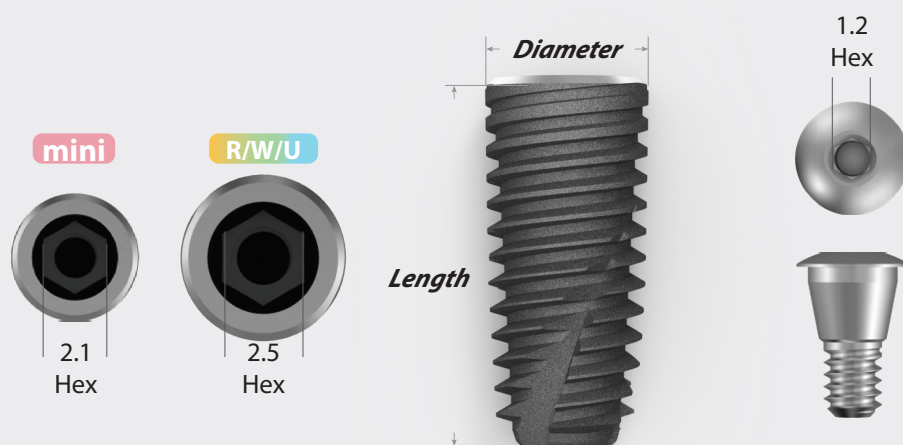

Nt2 **mini**

Length ● **D3.5**

8.5	NT2 35085 T
10	NT2 3510 T
11.5	NT2 35115 T
13	NT2 3513 T

* Use mini size abutment

- Mini
- Regular
- Wide
- Ultra-wide

Nt2 **R/W/U**


Length	● D4.0	● D4.5	● D5.0
7	NT2 4007 T	NT2 4507 T	NT2 5007 T
8.5	NT2 40085 T	NT2 45085 T	NT2 50085 T
10	NT2 4010 T	NT2 4510 T	NT2 5010 T
11.5	NT2 40115 T	NT2 45115 T	NT2 50115 T
13	NT2 4013 T	NT2 4513 T	NT2 5013 T

Length	● D5.5	● D6.0	● D6.5	● D7.0
7	NT2 5507 T	NT2 6007 T	NT2 6507 T	NT2 7007 T
8.5	NT2 55085 T	NT2 60085 T	NT2 65085 T	NT2 70085 T
10	NT2 5510 T	NT2 6010 T	NT2 6510 T	NT2 7010 T
11.5	NT2 55115 T	NT2 60115 T	NT2 65115 T	NT2 70115 T
13	NT2 5513 T	NT2 6013 T	NT2 6513 T	NT2 7013 T

* Use R/W/U size abutment

Submerged Abutment

- Mini
- Regular
- Wide
- Ultra-wide



Cover screw mini

Height

<i>0.5</i>	MICS 5005
<i>2</i>	MICS 5020

Cover screw R/W/U

Height


<i>0.5</i>	22HCSR 5005
<i>2</i>	22HCSR 5020

Method

Use 1.2 Hex hand driver
5~8Ncm Joining torque

Usage

Used to prevent foreign materials from entering after the fixture insertion



Healing abutment **mini**

	<i>GH</i>	<i>Height 3</i>	<i>Height 4</i>	<i>Height 5</i>	<i>Height 7</i>
D4.0	1	MHA 4013			
	2		MHA 4024	MHA 4025	
	3				MHA 4037
D4.5	1	MHA 4513			
	2		MHA 4524	MHA 4525	
	3				MHA 4537

Healing abutment **R/W/U**


	<i>GH</i>	<i>Height 3</i>	<i>Height 4</i>	<i>Height 5</i>	<i>Height 7</i>
D4.0	1	SHA 401030			
	2		SHA 402040	SHA 402050	
	3				SHA 403070
D4.5	1	SHA 451030			
	2		SHA 452040	SHA 452050	
	3				SHA 453070
D5.0	1	SHA 501030			
	2		SHA 502040	SHA 502050	
	3				SHA 503070
D5.5	1	SHA 551030			
	2		SHA 552040	SHA 552050	
	3				SHA 553070
D6.0	1	SHA 601030			
	2		SHA 602040	SHA 602050	
	3				SHA 603070
D6.5	1	SHA 651030			
	2		SHA 652040	SHA 652050	
	3				SHA 653070

Method

Use 1.2 Hex hand driver
5~8Ncm of joining torque

Usage

Used to protect the connecting part of the implant
Acts as the shape of the gingiva after surgery
Abutment is chosen according to the patient's gingival height.

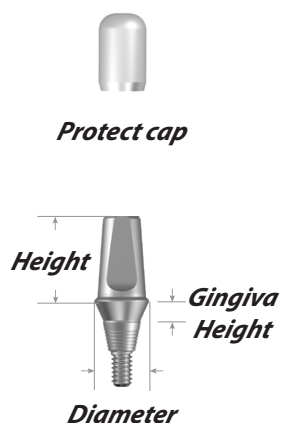

Solid abutment **mini**



	<i>H</i>	<i>GH 1</i>	<i>GH 2</i>	<i>GH 3</i>	<i>GH 4</i>	<i>GH 5</i>
	4	MSA 4014	MSA 4024	MSA 4034	MSA 4044	MSA 4054
D4.0	5.5	MSA 4015	MSA 4025	MSA 4035	MSA 4045	MSA 4055
	7	MSA 4017	MSA 4027	MSA 4037	MSA 4047	MSA 4057
	4	MSA 4514	MSA 4524	MSA 4534	MSA 4544	MSA 4554
D4.5	5.5	MSA 4515	MSA 4525	MSA 4535	MSA 4545	MSA 4555
	7	MSA 4517	MSA 4527	MSA 4537	MSA 4547	MSA 4557

Solid abutment

R/W/U



	<i>H</i>	<i>GH 1</i>	<i>GH 2</i>	<i>GH 3</i>	<i>GH 4</i>	<i>GH 5</i>
	4	SSA 401040	SSA 402040	SSA 403040	SSA 404040	SSA 405040
D4.0	5.5	SSA 401055	SSA 402055	SSA 403055	SSA 404055	SSA 405055
	7	SSA 401070	SSA 402070	SSA 403070	SSA 404070	SSA 405070
	4	SSA 451040	SSA 452040	SSA 453040	SSA 454040	SSA 455040
D4.5	5.5	SSA 451055	SSA 452055	SSA 453055	SSA 454055	SSA 455055
	7	SSA 451070	SSA 452070	SSA 453070	SSA 454070	SSA 455070
	4	SSA 501040	SSA 502040	SSA 503040	SSA 504040	SSA 505040
D5.0	5.5	SSA 501055	SSA 502055	SSA 503055	SSA 504055	SSA 505055
	7	SSA 501070	SSA 502070	SSA 503070	SSA 504070	SSA 505070
	4	SSA 551040	SSA 552040	SSA 553040	SSA 554040	SSA 555040
D5.5	5.5	SSA 551055	SSA 552055	SSA 553055	SSA 554055	SSA 555055
	7	SSA 551070	SSA 552070	SSA 553070	SSA 554070	SSA 555070
	4	SSA 601040	SSA 602040	SSA 603040	SSA 604040	SSA 605040
D6.0	5.5	SSA 601055	SSA 602055	SSA 603055	SSA 604055	SSA 605055
	7	SSA 601070	SSA 602070	SSA 603070	SSA 604070	SSA 605070
	4	SSA 651040	SSA 652040	SSA 653040	SSA 654040	SSA 655040
D6.5	5.5	SSA 651055	SSA 652055	SSA 653055	SSA 654055	SSA 655055
	7	SSA 651070	SSA 652070	SSA 653070	SSA 654070	SSA 655070

Method


Use 1.2 Hex torque driver
25~35Ncm joining torque

Components

Solid abutment + Protect cap

Usage


Used on the conventional cement type produced prosthesis
All-in-one abutment and screw structure



Transfer abutment Hex **mini**



	<i>H</i>	<i>GH 1</i>	<i>GH 2</i>	<i>GH 3</i>	<i>GH 4</i>	<i>GH 5</i>
D4.0	4	MTA 4014H	MTA 4024H	MTA 4034H	MTA 4044H	MTA 4054H
	5.5	MTA 4015H	MTA 4025H	MTA 4035H	MTA 4045H	MTA 4055H
	7	MTA 4017H	MTA 4027H	MTA 4037H	MTA 4047H	MTA 4057H
D4.5	4	MTA 4514H	MTA 4524H	MTA 4534H	MTA 4544H	MTA 4554H
	5.5	MTA 4515H	MTA 4525H	MTA 4535H	MTA 4545H	MTA 4555H
	7	MTA 4517H	MTA 4527H	MTA 4537H	MTA 4547H	MTA 4557H



Transfer abutment Non-Hex **mini**



	<i>H</i>	<i>GH 1</i>	<i>GH 2</i>	<i>GH 3</i>	<i>GH 4</i>	<i>GH 5</i>
D4.0	4	MTA 4014N	MTA 4024N	MTA 4034N	MTA 4044N	MTA 4054N
	5.5	MTA 4015N	MTA 4025N	MTA 4035N	MTA 4045N	MTA 4055N
	7	MTA 4017N	MTA 4027N	MTA 4037N	MTA 4047N	MTA 4057N
D4.5	4	MTA 4514N	MTA 4524N	MTA 4534N	MTA 4544N	MTA 4554N
	5.5	MTA 4515N	MTA 4525N	MTA 4535N	MTA 4545N	MTA 4555N
	7	MTA 4517N	MTA 4527N	MTA 4537N	MTA 4547N	MTA 4557N

Method


Use 1.2 Hex torque driver
25~35Ncm joining torque

Components

Transfer abutment + Abutment screw
Choice of variety of sizes according to gingival height

Usage

Conventional cement retained type abutment



Transfer abutment Hex R/W/U



	<i>H</i>	<i>GH 1</i>	<i>GH 2</i>	<i>GH 3</i>	<i>GH 4</i>	<i>GH 5</i>
D4.0	4	STA 401040H	STA 402040H	STA 403040H	STA 404040H	STA 405040H
	5.5	STA 401055H	STA 402055H	STA 403055H	STA 404055H	STA 405055H
	7	STA 401070H	STA 402070H	STA 403070H	STA 404070H	STA 405070H
D4.5	4	STA 451040H	STA 452040H	STA 453040H	STA 454040H	STA 455040H
	5.5	STA 451055H	STA 452055H	STA 453055H	STA 454055H	STA 455055H
	7	STA 451070H	STA 452070H	STA 453070H	STA 454070H	STA 455070H
D5.0	4	STA 501040H	STA 502040H	STA 503040H	STA 504040H	STA 505040H
	5.5	STA 501055H	STA 502055H	STA 503055H	STA 504055H	STA 505055H
	7	STA 501070H	STA 502070H	STA 503070H	STA 504070H	STA 505070H
D5.5	4	STA 551040H	STA 552040H	STA 553040H	STA 554040H	STA 555040H
	5.5	STA 551055H	STA 552055H	STA 553055H	STA 554055H	STA 555055H
	7	STA 551070H	STA 552070H	STA 553070H	STA 554070H	STA 555070H
D6.0	4	STA 601040H	STA 602040H	STA 603040H	STA 604040H	STA 605040H
	5.5	STA 601055H	STA 602055H	STA 603055H	STA 604055H	STA 605055H
	7	STA 601070H	STA 602070H	STA 603070H	STA 604070H	STA 605070H
D6.5	4	STA 651040H	STA 652040H	STA 653040H	STA 654040H	STA 655040H
	5.5	STA 651055H	STA 652055H	STA 653055H	STA 654055H	STA 655055H
	7	STA 651070H	STA 652070H	STA 653070H	STA 654070H	STA 655070H

Method


Use 1.2 Hex torque driver
25~35Ncm joining torque

Components

Transfer abutment + Abutment screw
Choice of variety of sizes according to gingival height

Usage

Conventional cement retained type abutment



Transfer abutment Non-Hex R/W/U



	<i>H</i>	<i>GH 1</i>	<i>GH 2</i>	<i>GH 3</i>	<i>GH 4</i>	<i>GH 5</i>
D4.0	4	STA 401040N	STA 402040N	STA 403040N	STA 404040N	STA 405040N
	5.5	STA 401055N	STA 402055N	STA 403055N	STA 404055N	STA 405055N
	7	STA 401070N	STA 402070N	STA 403070N	STA 404070N	STA 405070N
D4.5	4	STA 451040N	STA 452040N	STA 453040N	STA 454040N	STA 455040N
	5.5	STA 451055N	STA 452055N	STA 453055N	STA 454055N	STA 455055N
	7	STA 451070N	STA 452070N	STA 453070N	STA 454070N	STA 455070N
D5.0	4	STA 501040N	STA 502040N	STA 503040N	STA 504040N	STA 505040N
	5.5	STA 501055N	STA 502055N	STA 503055N	STA 504055N	STA 505055N
	7	STA 501070N	STA 502070N	STA 503070N	STA 504070N	STA 505070N
D5.5	4	STA 551040N	STA 552040N	STA 553040N	STA 554040N	STA 555040N
	5.5	STA 551055N	STA 552055N	STA 553055N	STA 554055N	STA 555055N
	7	STA 551070N	STA 552070N	STA 553070N	STA 554070N	STA 555070N
D6.0	4	STA 601040N	STA 602040N	STA 603040N	STA 604040N	STA 605040N
	5.5	STA 601055N	STA 602055N	STA 603055N	STA 604055N	STA 605055N
	7	STA 601070N	STA 602070N	STA 603070N	STA 604070N	STA 605070N
D6.5	4	STA 651040N	STA 652040N	STA 653040N	STA 654040N	STA 655040N
	5.5	STA 651055N	STA 652055N	STA 653055N	STA 654055N	STA 655055N
	7	STA 651070N	STA 652070N	STA 653070N	STA 654070N	STA 655070N

Method


Use 1.2 Hex torque driver
25~35Ncm joining torque

Components


Transfer abutment + Abutment screw
Choice of variety of sizes according to gingival height

Usage



Conventional cement retained type abutment



A Type



B Type



Angled abutment Hex **mini**



A Type	A	GH 1	GH 2	GH 3	GH 4	GH 5
D4.0	15	MAA 4011A	MAA 4021A	MAA 4031A	MAA 4041A	MAA 4051A
	25	MAA 4012A	MAA 4022A	MAA 4032A	MAA 4042A	MAA 4052A
D4.5	15	MAA 4511A	MAA 4521A	MAA 4531A	MAA 4541A	MAA 4551A
	25	MAA 4512A	MAA 4522A	MAA 4532A	MAA 4542A	MAA 4552A

B type	A	G/H 1	G/H 2	G/H 3	G/H 4	G/H 5
D4.0	15	MAA 4011B	MAA 4021B	MAA 4031B	MAA 4041B	MAA 4051B
	25	MAA 4012B	MAA 4022B	MAA 4032B	MAA 4042B	MAA 4052B
D4.5	15	MAA 4511B	MAA 4521B	MAA 4531B	MAA 4541B	MAA 4551B
	25	MAA 4512B	MAA 4522B	MAA 4532B	MAA 4542B	MAA 4552B

H = 7mm

Angled abutment Non-Hex **mini**



	A	GH 1	GH 2	GH 3	GH 4	GH 5
D4.0	15	MAA 4011N	MAA 4021N	MAA 4031N	MAA 4041N	MAA 4051N
	25	MAA 4012N	MAA 4022N	MAA 4032N	MAA 4042N	MAA 4052N
D4.5	15	MAA 4511N	MAA 4521N	MAA 4531N	MAA 4541N	MAA 4551N
	25	MAA 4512N	MAA 4522N	MAA 4532N	MAA 4542N	MAA 4552N

H = 7mm

Method




Use 1.2 Hex torque driver
25~35Ncm joining torque

Components

Angled abutment + Abutment screw
15° / 25° composition

Usage

Conventional cement retained type abutment
Used in revising the fixture's path
Used in cases when the prosthesis' path needs to be adjusted

**A Type****B Type****Angled abutment Hex****R/W/U**

A Type	A	GH 1	GH 2	GH 3	GH 4	GH 5
D4.0	15	SAA 401015A	SAA 402015A	SAA 403015A	SAA 404015A	SAA 405015A
	25	SAA 401025A	SAA 402025A	SAA 403025A	SAA 404025A	SAA 405025A
D4.5	15	SAA 451015A	SAA 452015A	SAA 453015A	SAA 454015A	SAA 455015A
	25	SAA 451025A	SAA 452025A	SAA 453025A	SAA 454025A	SAA 455025A
D5.0	15	SAA 501015A	SAA 502015A	SAA 503015A	SAA 504015A	SAA 505015A
	25	SAA 501025A	SAA 502025A	SAA 503025A	SAA 504025A	SAA 505025A
D5.5	15	SAA 551015A	SAA 552015A	SAA 553015A	SAA 554015A	SAA 555015A
	25	SAA 551025A	SAA 552025A	SAA 553025A	SAA 554025A	SAA 555025A
D6.0	15	SAA 601015A	SAA 602015A	SAA 603015A	SAA 604015A	SAA 605015A
	25	SAA 601025A	SAA 602025A	SAA 603025A	SAA 604025A	SAA 605025A
D6.5	15	SAA 651015A	SAA 652015A	SAA 653015A	SAA 654015A	SAA 655015A
	25	SAA 651025A	SAA 652025A	SAA 653025A	SAA 654025A	SAA 655025A

B type	A	GH 1	GH 2	GH 3	GH 4	GH 5
D4.0	15	SAA 401015B	SAA 402015B	SAA 403015B	SAA 404015B	SAA 405015B
	25	SAA 401025B	SAA 402025B	SAA 403025B	SAA 404025B	SAA 405025B
D4.5	15	SAA 451015B	SAA 452015B	SAA 453015B	SAA 454015B	SAA 455015B
	25	SAA 451025B	SAA 452025B	SAA 453025B	SAA 454025B	SAA 455025B
D5.0	15	SAA 501015B	SAA 502015B	SAA 503015B	SAA 504015B	SAA 505015B
	25	SAA 501025B	SAA 502025B	SAA 503025B	SAA 504025B	SAA 505025B
D5.5	15	SAA 551015B	SAA 552015B	SAA 553015B	SAA 554015B	SAA 555015B
	25	SAA 551025B	SAA 552025B	SAA 553025B	SAA 554025B	SAA 555025B
D6.0	15	SAA 601015B	SAA 602015B	SAA 603015B	SAA 604015B	SAA 605015B
	25	SAA 601025B	SAA 602025B	SAA 603025B	SAA 604025B	SAA 605025B
D6.5	15	SAA 651015B	SAA 652015B	SAA 653015B	SAA 654015B	SAA 655015B
	25	SAA 651025B	SAA 652025B	SAA 653025B	SAA 654025B	SAA 655025B

H = 7mm**Method**


Use 1.2 Hex torque driver
25~35Ncm joining torque

Components

Angled abutment + Abutment screw
15° / 25° composition

Usage

Conventional cement retained type abutment
Used in revising the fixture's path
Used in cases when the prosthesis' path needs to be adjusted



Angled abutment Non-Hex R/W/U



	<i>A</i>	<i>GH 1</i>	<i>GH 2</i>	<i>GH 3</i>	<i>GH 4</i>	<i>GH 5</i>
D4.0	15	SAA 401015N	SAA 402015N	SAA 403015N	SAA 404015N	SAA 405015N
	25	SAA 401025N	SAA 402025N	SAA 403025N	SAA 404025N	SAA 405025N
D4.5	15	SAA 451015N	SAA 452015N	SAA 453015N	SAA 454015N	SAA 455015N
	25	SAA 451025N	SAA 452025N	SAA 453025N	SAA 454025N	SAA 455025N
D5.0	15	SAA 501015N	SAA 502015N	SAA 503015N	SAA 504015N	SAA 505015N
	25	SAA 501025N	SAA 502025N	SAA 503025N	SAA 504025N	SAA 505025N
D5.5	15	SAA 551015N	SAA 552015N	SAA 553015N	SAA 554015N	SAA 555015N
	25	SAA 551025N	SAA 552025N	SAA 553025N	SAA 554025N	SAA 555025N
D6.0	15	SAA 601015N	SAA 602015N	SAA 603015N	SAA 604015N	SAA 605015N
	25	SAA 601025N	SAA 602025N	SAA 603025N	SAA 604025N	SAA 605025N
D6.5	15	SAA 651015N	SAA 652015N	SAA 653015N	SAA 654015N	SAA 655015N
	25	SAA 651025N	SAA 652025N	SAA 653025N	SAA 654025N	SAA 655025N

H = 7mm

Method


Use 1.2 Hex torque driver
25~35Ncm joining torque

Components

Angled abutment + Abutment screw
15° / 25° composition

Usage


Conventional cement retained type abutment
Used in revising the fixture's path
Used in cases when the prosthesis' path needs to be adjusted

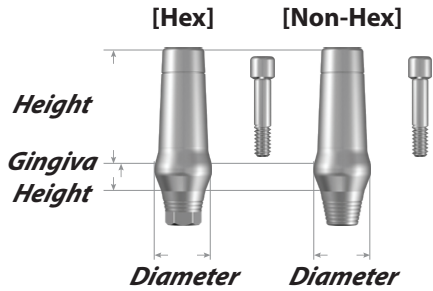

Milling abutment **mini**



	GH 2		GH 4	
	Hex	Non-Hex	Hex	Non-Hex
D4.5	MMA 4529H	MMA 4529N	MMA 4549H	MMA 4549N

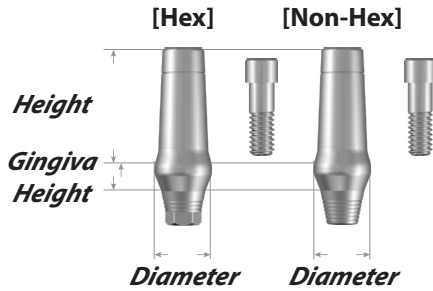

Milling abutment **R/W/U**



	GH 2		GH 4	
	Hex	Non-Hex	Hex	Non-Hex
D5.0	SMA 5029H	SMA 5029N	SMA 5049H	SMA 5049N
D5.5	SMA 5529H	SMA 5529N	SMA 5549H	SMA 5549N
D6.0	SMA 6029H	SMA 6029N	SMA 6049H	SMA 6049N

H = 9mm

Method


Use 1.2 Hex torque driver
25~35Ncm joining torque

Components

Milling abutment + Abutment screw

Usage


Used in cases when the height or margin of abutment needs to be customized

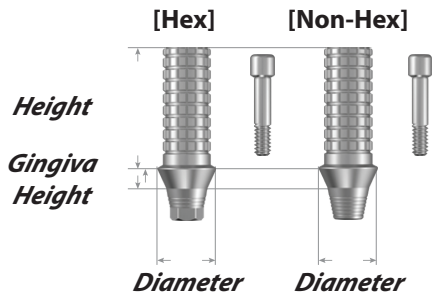

Temporary abutment **mini**



	GH 2		GH 4	
	Hex	Non-Hex	Hex	Non-Hex
D4.5	MTPA 452H	MTPA 452N	MTPA 454H	MTPA 454N

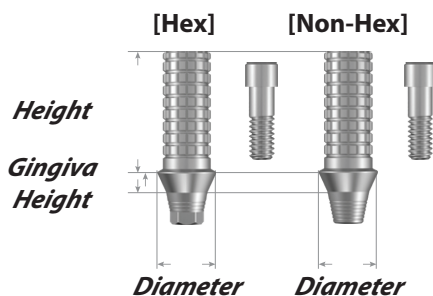

Temporary abutment **R/W/U**



	GH 2		GH 4	
	Hex	Non-Hex	Hex	Non-Hex
D5.0	STPA 502H	STPA 502N	STPA 504H	STPA 504N

H = 10mm

Method


Use 1.2 Hex torque driver
25~35Ncm joining torque

Components

Temporary abutment + Abutment screw

Usage

Used in cases making the temporary prosthesis



Solid lab analog M/R/W/U

	<i>Height 4</i>	<i>Height 5.5</i>	<i>Height 7</i>
D4.0	S-SLA 4040	S-SLA 4055	S-SLA 4070
D4.5	S-SLA 4540	S-SLA 4555	S-SLA 4570
D5.0	S-SLA 5040	S-SLA 5055	S-SLA 5070
D5.5	S-SLA 5540	S-SLA 5555	S-SLA 5570
D6.0	S-SLA 6040	S-SLA 6055	S-SLA 6070
D6.5	S-SLA 6540	S-SLA 6555	S-SLA 6570


Method

Used on solid abutment features

Used to produce the model for solid Impression coping connection pick up inside the oral cavity

Usage

Solid abutment is materialized in the oral cavity on the working replica



Solid impression coping M/R/W/U

	<i>Height 4</i>	<i>Height 5.5</i>	<i>Height 7</i>
D4.0	S-IC 4040	S-IC 4055	S-IC 4070
D4.5	S-IC 4540	S-IC 4555	S-IC 4570
D5.0	S-IC 5040	S-IC 5055	S-IC 5070
D5.5	S-IC 5540	S-IC 5555	S-IC 5570
D6.0	S-IC 6040	S-IC 6055	S-IC 6070
D6.5	S-IC 6540	S-IC 6555	S-IC 6570

Method

Used on solid Abutment features

Integration of existing positioning cylinder and Impression Cap



Fixture lab analog **mini**

M-FLA 35

Fixture lab analog **R/W/U**

S-FLA 45

Method

For Gt2/Nt2


Used on abutment features

Used to produce the model for solid Impression coping


Connection pick up inside the oral cavity

Usage

Fixture is materialized in the oral cavity on the working replica



[Non-Hex]



Impression coping (Transfer) **mini**

	<i>Length 11</i>		<i>Length 15</i>	
	<i>Hex</i>	<i>Non-Hex</i>	<i>Hex</i>	<i>Non-Hex</i>
D4.0	M-ICT 4011H	M-ICT 4011N	M-ICT 4015H	M-ICT 4015N

Impression coping (Transfer) **R/W/U**

	<i>Length 11</i>		<i>Length 15</i>	
	<i>Hex</i>	<i>Non-Hex</i>	<i>Hex</i>	<i>Non-Hex</i>
D4.5	S-ICT 4511H	S-ICT 4511N	S-ICT 4515H	S-ICT 4515N

Method

Use 1.2 Hex hand driver

Components


Impression coping + Guide pin (2 pieces)

11mm / 15mm Coping size



Usage

Existing tray is used

[Hex]



[Non-Hex]



Impression coping (Pick-up) **mini**

	<i>Length 10</i>		<i>Length 15</i>	
	<i>Hex</i>	<i>Non-Hex</i>	<i>Hex</i>	<i>Non-Hex</i>
D4.0	M-ICP 4010H	M-ICP 4010N	M-ICP 4015H	M-ICP 4015N

Impression coping (Pick-up) **R/W/U**

	<i>Length 10</i>		<i>Length 15</i>	
	<i>Hex</i>	<i>Non-Hex</i>	<i>Hex</i>	<i>Non-Hex</i>
D4.0	S-ICP 4010H	S-ICP 4010N	S-ICP 4015H	S-ICP 4015N
D4.5	S-ICP 4510H	S-ICP 4510N	S-ICP 4515H	S-ICP 4515N
D5.0	S-ICP 5010H	S-ICP 5010N	S-ICP 5015H	S-ICP 5015N
D5.5	S-ICP 5510H	S-ICP 5510N	S-ICP 5515H	S-ICP 5515N
D6.0	S-ICP 6010H	S-ICP 6010N	S-ICP 6015H	S-ICP 6015N

Impression coping Guide pin (Pick-up) **mini**

<i>Length 10</i>	<i>Length 15</i>	<i>Length 20</i>
M-PG 100	M-PG 150	M-PG 200

Impression coping Guide pin (Pick-up) **R/W/U**

<i>Length 10</i>	<i>Length 15</i>	<i>Length 20</i>
S-PG 100	S-PG 150	S-PG 200

Method


Use hand or 1.2 Hex hand driver

Components

Impression coping + Guide pin
10mm/15mm/20mm Guide pin size

Usage


Use of custom tray
Increases the ease of various guide pin size



UCLA Abutment **mini**

	<i>Hex</i>	<i>Non-Hex</i>
D4.0	MUT 402H	MUT 402N


GH = 2mm



UCLA Abutment **R/W/U**


	<i>Hex</i>	<i>Non-Hex</i>
D4.5	SUT 452H	SUT 452N

GH = 2mm



Plastic Cylinder **mini**


	<i>Hex</i>	<i>Non-Hex</i>
D4.0	M-PSC 40H	M-PSC 40N




Plastic Cylinder **R/W/U**

	<i>Hex</i>	<i>Non-Hex</i>
D4.5	S-PSC 45H	S-PSC 45N

Multi-unit system

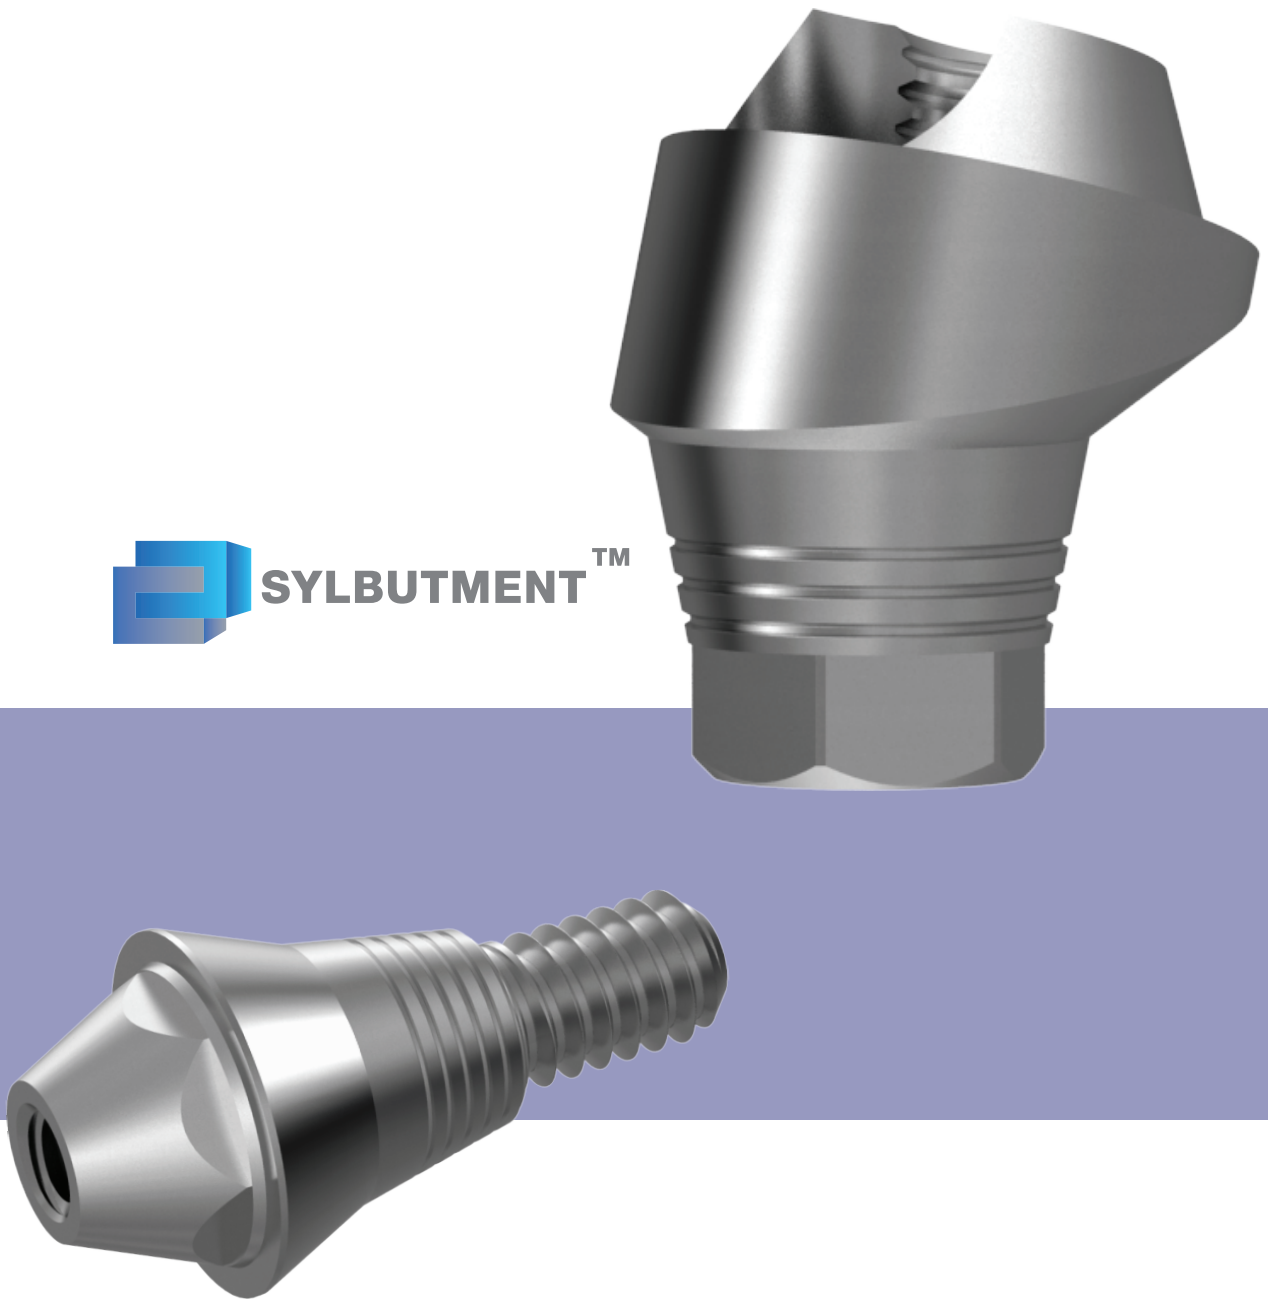


Multi-unit system Flow chart

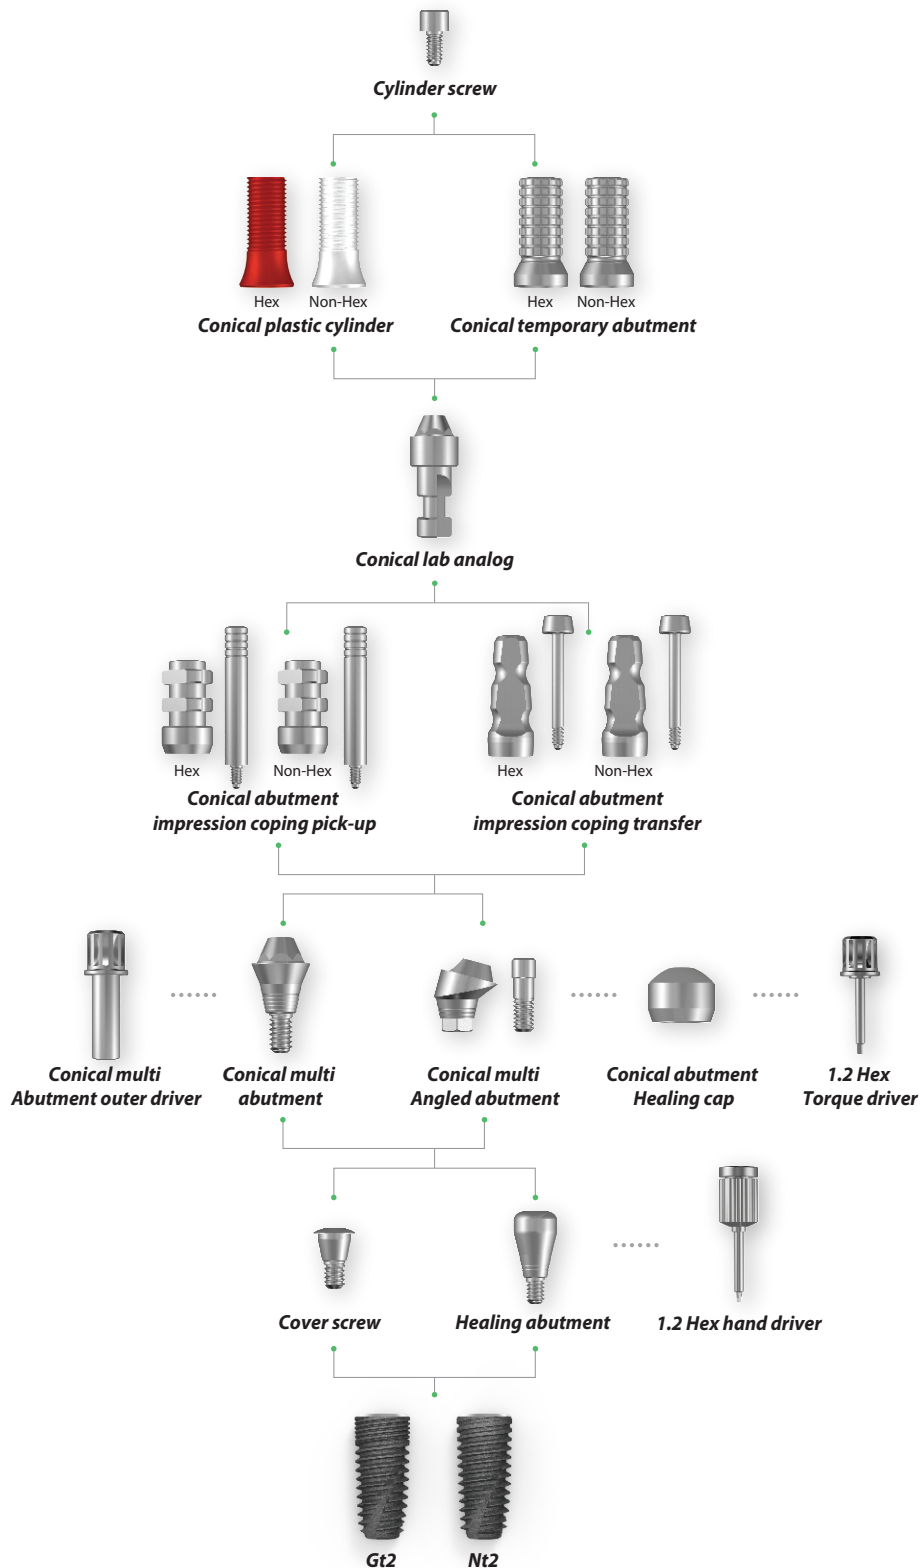

Multi-unit Submerged abutment

- Mini
- Regular
- Wide
- Ultra-wide

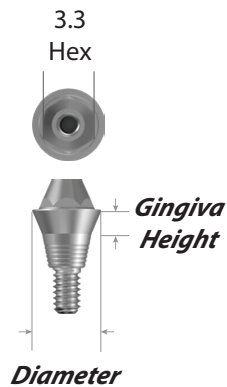

Conical multi abutment **mini**




	<i>GH 1</i>	<i>GH 2</i>	<i>GH 3</i>	<i>GH 4</i>	<i>GH 5</i>
D4.8	MCMA 4810	MCMA 4820	MCMA 4830	MCMA 4840	MCMA 4850

Conical multi abutment **R/W/U**



	<i>GH 1</i>	<i>GH 2</i>	<i>GH 3</i>	<i>GH 4</i>	<i>GH 5</i>
D4.8	CMA 4810	CMA 4820	CMA 4830	CMA 4840	CMA 4850

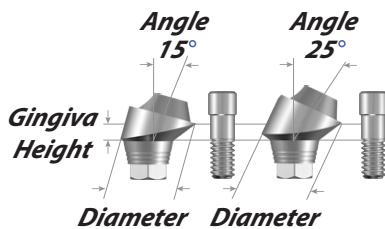

Conical multi angled abutment **mini**




	<i>A</i>	<i>GH 1.5</i>	<i>GH 2.5</i>
D4.8	15	MCMAA 481515 H	MCMAA 482515 H
	25	MCMAA 481525 H	MCMAA 482525 H

Conical multi angled abutment **R/W/U**



	<i>A</i>	<i>GH 1.5</i>	<i>GH 2.5</i>
D4.8	15	CMAA 481515 H	CMAA 482515 H
	25	CMAA 481525 H	CMAA 482525 H



Conical abutment healing cap **M/R/W/U**

	<i>H 6.0</i>
D4.8	CAHC 600

Conical multi abutment outer driver



	<i>Short (8mm)</i>	<i>Long (15mm)</i>
Hex 3.3	RHV 33 S	RHV 33 L

Diameter




Conical lab analog M/R/W/U

D4.8 CLA 48

[Hex]

[Non-Hex]

Length



Conical temporary abutment M/R/W/U


Length 12

	<i>Hex</i>	<i>Non-Hex</i>
D4.8	CTPA 48 H	CTPA 48 N

[Hex]

[Non-Hex]

Length



Conical plastic cylinder M/R/W/U


Length 12

	<i>Hex</i>	<i>Non-Hex</i>
D4.8	CPSC 48 H	CPSC 48 N

[Hex]

[Non-Hex]

Length

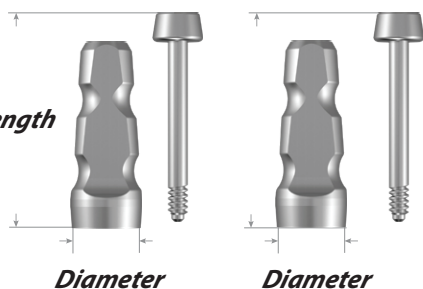

Conical abutment impression coping (Transfer) M/R/W/U

Length 11


Length 15

	<i>Hex</i>	<i>Non-Hex</i>	<i>Hex</i>	<i>Non-Hex</i>
D4.8	CAICT 4811 H	CAICT 4811 N	CAICT 4815 H	CAICT 4815 N

[Hex]

[Non-Hex]

Length

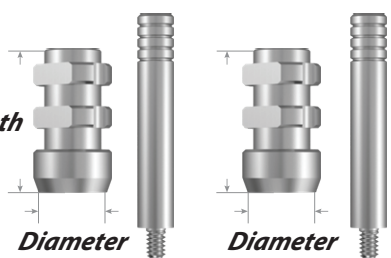

Conical abutment Impression coping (Pick up) M/R/W/U

Length 10

Length 15

	<i>Hex</i>	<i>Non-Hex</i>	<i>Hex</i>	<i>Non-Hex</i>
D4.8	CAICP 4810 H	CAICP 4810 N	CAICP 4815 H	CAICP 4815 N

Internal Fixture

Vt1

Connection


3.1 Octa indentation and 8 degree Morse Taper. (Upper part is compatible with ITI)



Esthetic Type


Collar 1.8 Esthetic Type of Machined Surface

Dual Thread



As 0.8mm pitch of dual thread type, the surgery time is reduced. (1.6mm per 1 rotation)

RBM Surface



Surface areas are increased through blasting by highly biocompatible Calcium-Phosphate Media.

Main Thread

When the fixture is inserted into the implant bed, the conical shape and lower deep thread of the fixture increase stability and make immediate loading possible.

Cutting Edge




When placing the implants, the cutting edge of the Twist Type increases Self Tapping ability and minimizes Bone resistance.



Apex


Apex has the dimension of $D(\text{fixture diameter}) - 0.7\text{mm}$ and the body shape has the overall tapered one.

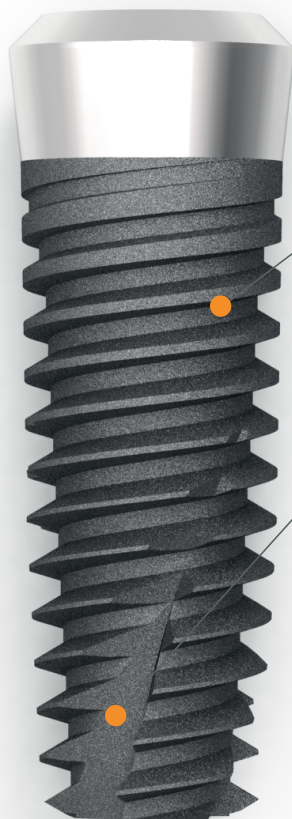

St1

Connection

3.1 Octa indentation and 8 degree Morse Taper. (Upper part is compatible with IT1)

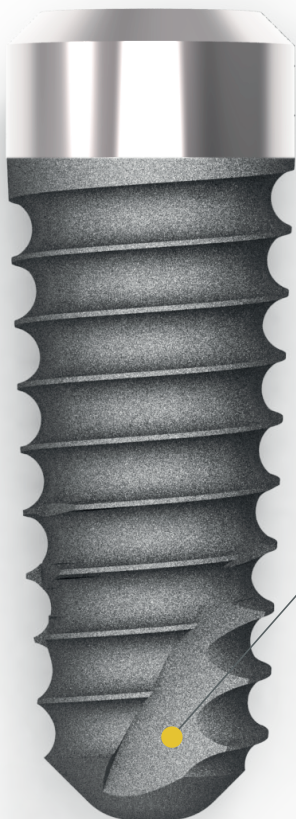


Esthetic Type

Collar 1.8 Esthetic Type of Machined Surface

Thread Design


As a form of streamline Round Thread, it is effective in stress distribution and prevents bone from the crack caused by the chewing forces.

Fin Type Design



When placing implants, initial guiding ability, stability and bone condensing effect is excellent.

RBM Surface



Surface areas are increased through blasting by highly biocompatible Calcium-Phosphate Media.

Simple Surgical Procedures

Due to the exterior Thread Taper design, initial penetration is excellent and surgical operation and drilling time is reduced.

Reverse Engaging Flute





When placing implants, it gradually expands bones, inducing Self Engaging.

Apex


Apex has the dimension of $D(\text{fixture diameter}) - 0.7\text{mm}$ and the body shape has the overall tapered one.

Internal system Flow chart

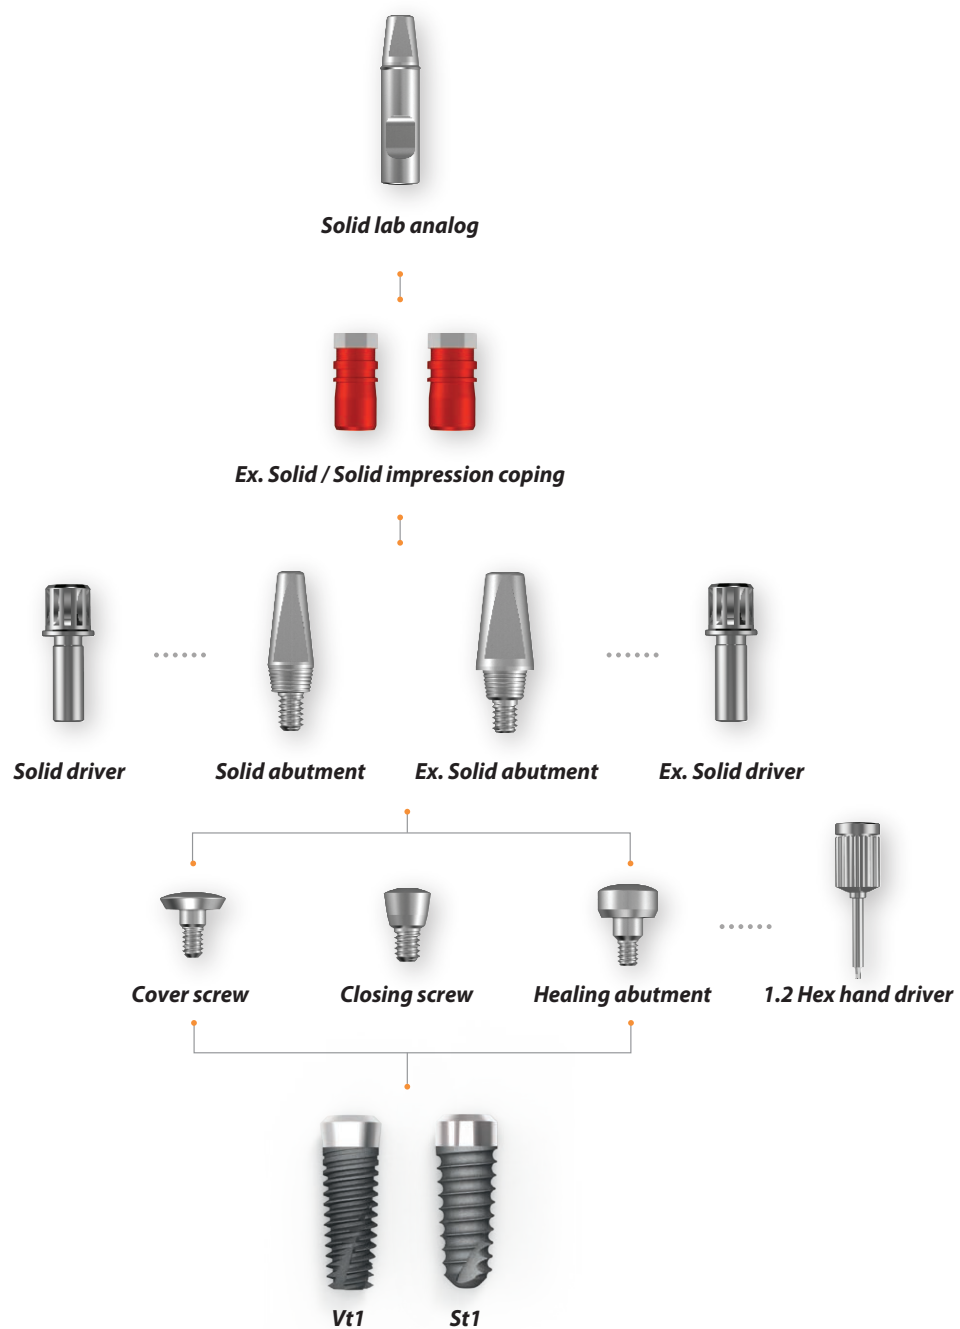

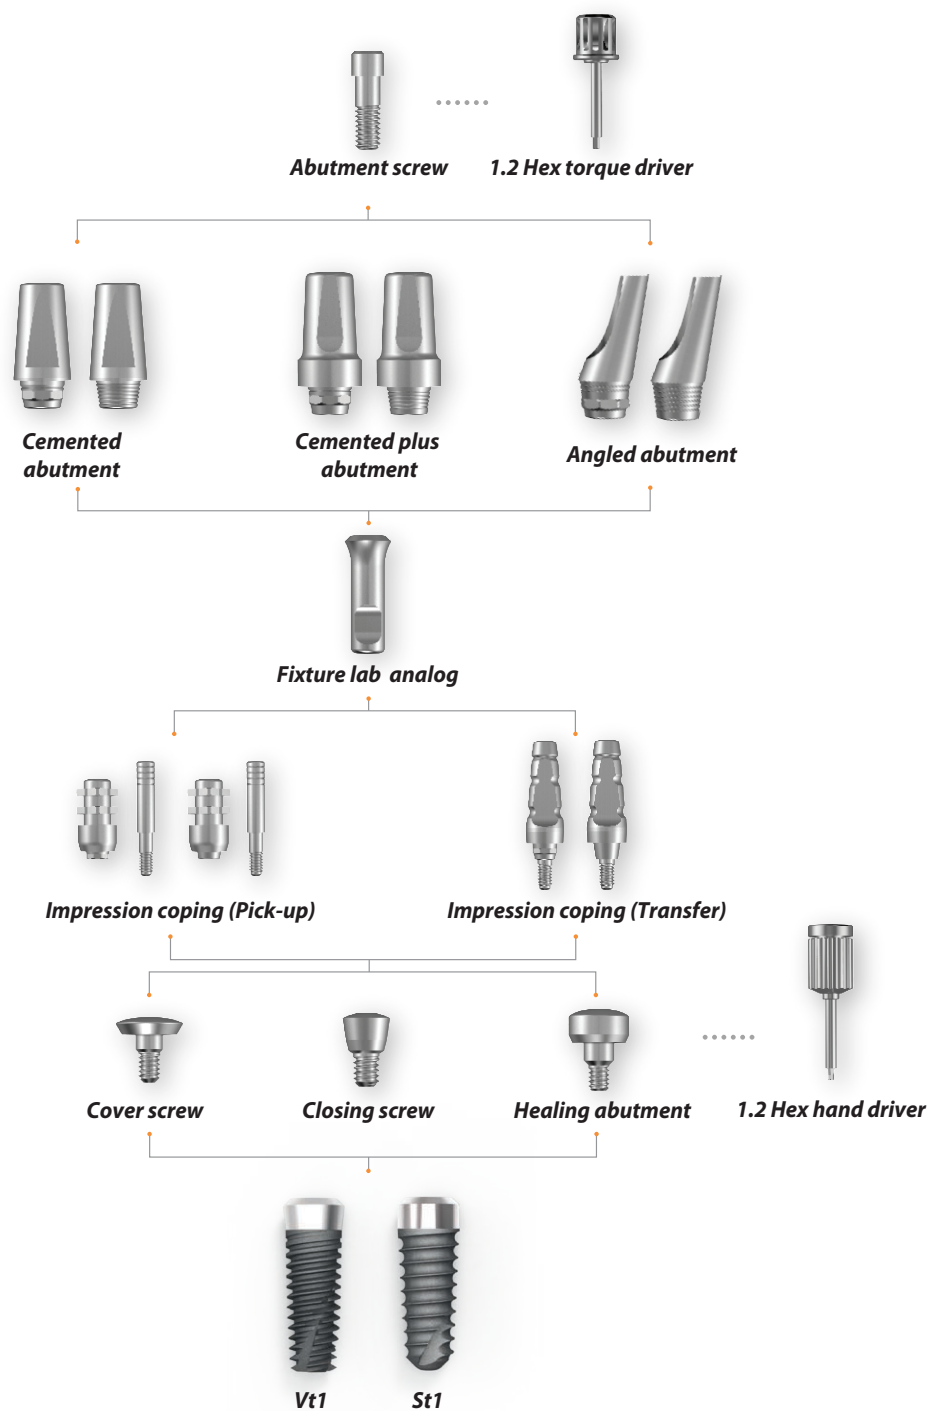

Internal Fixture

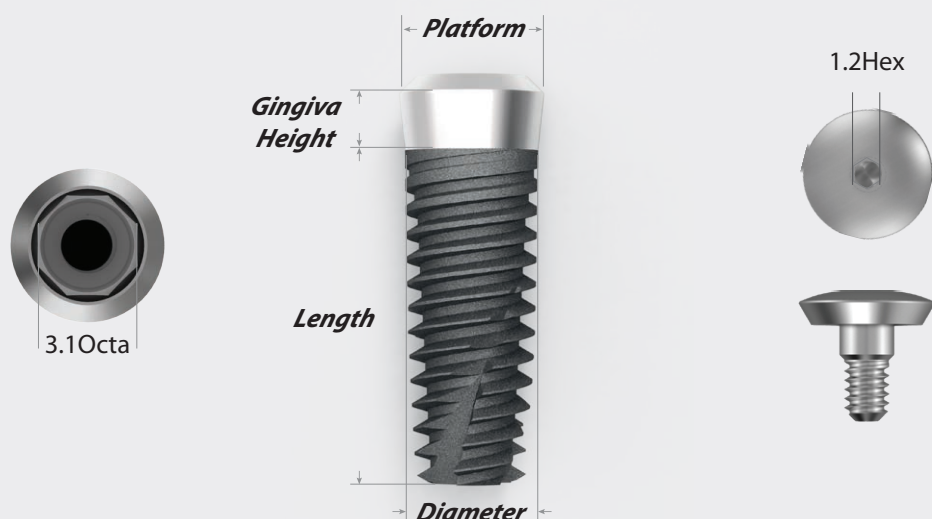


● Regular
● Wide

Vt1

Gingiva Height = 1.8mm

<i>Platform 4.8</i>			
<i>Length</i>	● <i>D4.1</i>	● <i>D4.4</i>	● <i>D4.8</i>
7	VT14107 T	VT14407 T	VT14807 T
8.5	VT141085 T	VT144085 T	VT148085 T
10	VT14110 T	VT14410 T	VT14810 T
11.5	VT141115 T	VT144115 T	VT148115 T
13	VT14113 T	VT14413 T	VT14813 T

<i>Platform 6.5</i>		
<i>Length</i>	● <i>D5.3</i>	● <i>D5.8</i>
7	VT1W 5307 T	VT1W 5807 T
8.5	VT1W 53085 T	VT1W 58085 T
10	VT1W 5310 T	VT1W 5810 T
11.5	VT1W 53115 T	VT1W 58115 T
13	VT1W 5313 T	VT1W 5813 T

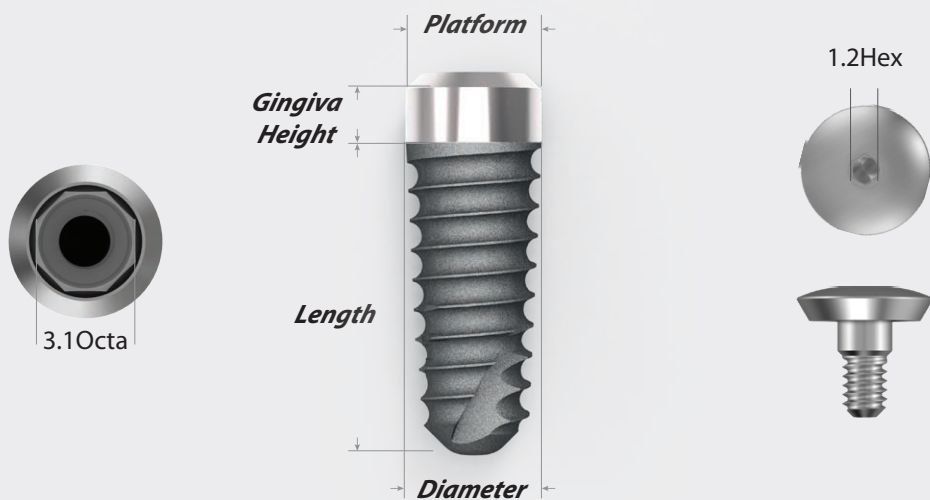

● Regular
● Wide


St1

Gingiva Height = 1.8mm

<i>Platform 4.8</i>			
<i>Length</i>	● <i>D4.1</i>	● <i>D4.4</i>	● <i>D4.8</i>
7	ST1 4107 T	ST1 4407 T	ST1 4807 T
8.5	ST1 41085 T	ST1 44085 T	ST1 48085 T
10	ST1 4110 T	ST1 4410 T	ST1 4810 T
11.5	ST1 41115 T	ST1 44115 T	ST1 48115 T
13	ST1 4113 T	ST1 4413 T	ST1 4813 T

<i>Platform 6.5</i>		
<i>Length</i>	● <i>D5.3</i>	● <i>D5.8</i>
7	ST1W 5307 T	ST1W 5807 T
8.5	ST1W 53085 T	ST1W 58085 T
10	ST1W 5310 T	ST1W 5810 T
11.5	ST1W 53115 T	ST1W 58115 T
13	ST1W 5313 T	ST1W 5813 T

Internal Abutment



Cover screw


	<i>Height 1.5</i>
P4.8	ICS 001
P6.5	ICSW 001

Method

Use 1.2 Hex hand driver
5~8Ncm of joining torque

Usage

Used to protect the connecting part of the implant



Closing screw


	<i>Height 0.5</i>
P4.8	ICS 002
P6.5	ICSB 002

Method

Use 1.2 Hex hand driver
5~8Ncm of joining torque

Usage

Used to protect the connecting part of the implant
Used to restrict the cases of adjoining space



Healing abutment

	<i>Height 2</i>	<i>Height 3</i>	<i>Height 4</i>	<i>Height 5</i>
P4.8	IH 200	IH 300	IH 400	IH 500
P6.5	IHW 200	IHW 300	IHW 400	IHW 500

Method

Use 1.2 Hex hand driver
5~8Ncm of joining torque

Usage

Used to protect the connecting part of the implant
Acts as the shape of the gingiva after surgery
Abutment is chosen according to the patient's gingival height

**Protect cap****Height****Solid abutment**

	<i>Height 4</i>	<i>Height 5.5</i>	<i>Height 7</i>
P4.8	SSA 440	SSA 455	SSA 470
P6.5	SSA 6040	SSA 6055	SSA 6070

Method**P4.8 :** Use Solid abutment driver**P6.5 :** Use 1.2 Hex torque driver
25~35Ncm of joining torque**Components**

Solid abutment + Protect cap


UsageUsed on the conventional cement type produced prosthesis
All-in-one abutment and screw structure**Protect cap****Height****Ex. Solid abutment**

	<i>Height 4</i>	<i>Height 5.5</i>	<i>Height 7</i>
P4.8	SESA 440	SESA 455	SESA 470
P6.5	SESA 6540	SESA 6555	SESA 6570

Method**P4.8 :** Use Ex. solid driver**P6.5 :** Use 1.2 Hex torque driver
25~35Ncm of joining torque**Components**

Ex. Solid abutment + Protect cap

UsageUsed on the conventional cement type produced prosthesis
All-in-one abutment and screw structure
Because it is bigger than solid type this is used in cases
where there are free spaces in the adjoining teeth

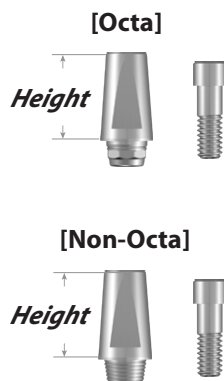

Cemented abutment



	<i>H</i>	<i>Octa</i>	<i>Non-Octa</i>
<i>P4.8</i>	<i>4</i>	SEOA 4304O	SEOA 4304N
	<i>5.5</i>	SEOA 4305O	SEOA 4305N
	<i>7</i>	SEOA 4307O	SEOA 4307N
<i>p6.5</i>	<i>4</i>	SEOA 5504O	SEOA 5504N
	<i>5.5</i>	SEOA 5505O	SEOA 5505N
	<i>7</i>	SEOA 5507O	SEOA 5507N

Method


Use 1.2 Hex torque driver
25~35Ncm joining torque

Components

Cemented abutment + Abutment screw
Implant connection by octa/non-octa composition is used according to surgery method and produced prosthesis

Usage

Conventional cement type prosthesis is used

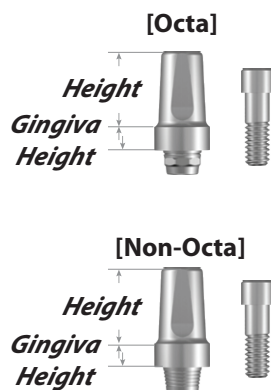

Cemented plus abutment



	<i>GH</i>	<i>Octa</i>	<i>Non-Octa</i>
P4.8	2	SEOA 4826O	SEOA 4826N
	4	SEOA 4846O	SEOA 4846N
P6.5	2	SEOA 6526O	SEOA 6526N
	4	SEOA 6546O	SEOA 6546N

H = 6mm

Method



Use 1.2 Hex torque driver
25~35Ncm joining torque

Components

Cemented plus abutment + Abutment screw
GH2, GH4 choice of sizes as gingival height

Usage

Conventional cement type prosthesis is used



Angled abutment



	<i>Angle</i>	<i>Octa</i>	<i>Non-Octa</i>
P4.8	15	SSAA 4715O	SSAA 4715N
	25	SSAA 4725O	SSAA 4725N
P6.5	15	SSAA 6715O	SSAA 6715N
	25	SSAA 6725O	SSAA 6725N

H = 7mm

Method


Use 1.2 Hex torque driver
25~35Ncm joinin torque

Components

Angled abutment + Abutment screw
15° / 25°

Usage

Conventional cement retained type abutment
Used in revising the fixture's path
Used in cases when the prosthesis' path needs to be adjusted



Solid lab analog


	<i>Height 4</i>	<i>Height 5.5</i>	<i>Height 7</i>
P4.8	SLA 440	SLA 455	SLA 470
P6.5	SLA 6540	SLA 6555	SLA 6570

Method

Used on Solid abutment features

Usage

Solid abutment is materialized in the oral cavity on the working replica



Ex. Solid lab analog


	<i>Height 4</i>	<i>Height 5.5</i>	<i>Height 7</i>
P4.8	ESLA 440	ESLA 455	ESLA 470
P6.5	ESLA 6540	ESLA 6555	ESLA 6570

Method

Used on Ex. Solid abutment features

Usage

Ex. Solid abutment is materialized in the oral cavity on the working replica




Solid Impression coping

	<i>Height 4</i>	<i>Height 5.5</i>	<i>Height 7</i>
P4.8	ICR 440	ICR 455	ICR 470
P6.5	ICW 6540	ICW 6555	ICW 6570

Method

Used on Solid abutment features

Integration of existing positioning cylinder and impression cap



Ex. Solid Impression coping

	<i>Height 4</i>	<i>Height 5.5</i>	<i>Height 7</i>
P4.8	EICR 440	EICR 455	EICR 470
P6.5	EICW 6540	EICW 6555	EICW 6570

Method

Used on Ex. Solid abutment features

Integration of existing positioning cylinder and impression cap



Fixture lab analog

	<i>Octa</i>
P4.8	FLA 48
P6.5	FLA 65

Method


For Vt1/St1

Used on abutment features


Usage

Fixture is materialized in the oral cavity on the working replica

[Octa]



[Non-Octa]



Impression coping (Transfer)

	<i>L</i>	<i>Octa</i>	<i>Non-Octa</i>
P4.8	11	TEOIC 4811O	TEOIC 4811N
	15	TEOIC 4815O	TEOIC 4815N
P6.5	11	TEOIC 6511O	TEOIC 6511N
	15	TEOIC 6515O	TEOIC 6515N

Method

Use 1.2 Hex hand driver


Components

Impression coping + Guide pin (2 pieces)
11mm / 15mm coping size


Usage

Existing tray is used

[Octa]



[Non-Octa]



Impression coping (Pick-up)

	<i>Octa</i>	<i>Non-Octa</i>
P4.8	EOI 4855O	EOI 4855N
P6.5	EOI 6570O	EOI 6570N

Impression coping Guide pin (Pick-up)

<i>Length 10</i>	<i>Length 15</i>	<i>Length 20</i>
EOG 100	EOG 150	EOG 200

Method

Use 1.2 Hex hand driver


Components

Impression coping + Guide pin
10mm/15mm/20mm Guide pin size

Usage

Use of custom tray
Increases the ease of various guide pin size

Common components of Surgical kits



Guide drill

	<i>Diameter</i>	<i>Length</i>
<i>GDR 20B</i>	2.0	15


- Easily forms the first hole in the initial drilling
- Marks the direction of the initial drilling in the cortical bone structure
- Only the triangular tip of the drill bit is used
- Bone density is assessed through the guide drill



Drill extention

DRE 002

- To extend the length of the used drills and other surgical equipment handpieces.



Parallel pin

	<i>D1</i>	<i>D2</i>	<i>D3</i>	<i>L</i>
<i>TPP 50</i>	5.0	2.8	2.2	10


- Confirms the direction and distance in bone preparation.
- Confirms the distance of spaces in multi-insertions.



Torque wrench


TRW 400 B

- Used when inserting the fixture and fastening the screw
- Possible 15/25/35N tool adjustment




Fixture driver Hex **mini**

		<i>Hex</i>
<i>For Handpiece</i>	<i>MMHL 002S</i>	2.1
	<i>MMHL 002L</i>	2.1
<i>For Torque wrench</i>	<i>RMHL 002S</i>	2.1
	<i>RMHL 002L</i>	2.1



Fixture driver Hex **R/W/U**

		<i>Hex</i>
<i>For Handpiece</i>	<i>MHL 002S</i>	2.5
	<i>MHL 002L</i>	2.5
<i>For Torque wrench</i>	<i>RHL 002S</i>	2.5
	<i>RHL 002L</i>	2.5



Fixture driver Octa **R/W/U**


		<i>Octa</i>
<i>For Handpiece</i>	<i>MOL 002S</i>	3.1
	<i>MOL 002L</i>	3.1
<i>For Torque wrench</i>	<i>ROL 002S</i>	3.1
	<i>ROL 002L</i>	3.1

For Handpiece

- Fastened with handpiece engine
- For Handpiece is used to insert and fasten the fixture
- Designed to prevent dropping when picking up the fixture to be fastened

For Torque wrench

- Fastened with torque wrench
- For Torque Wrench is used to insert and fasten the fixture
- Designed to prevent dropping when picking up the fixture to be fastened.

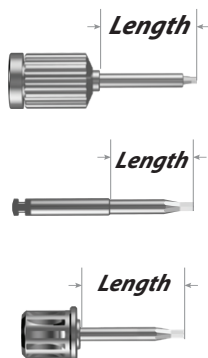

1.2 Hex driver

		<i>Length</i>	<i>Hex</i>
<i>Hand driver</i>	<i>THV 12SB</i>	8	1.2
	<i>THV 12LB</i>	15	1.2
<i>Machine driver</i>	<i>MHV 12SB</i>	8	1.2
	<i>MHV 12LB</i>	15	1.2
<i>Torque driver</i>	<i>RHV 12SB</i>	8	1.2
	<i>RHV 12LB</i>	15	1.2

Hand driver

- Hand driver is used when manually fastening the fixture with the joined abutment and screw


Machine driver

- Driver for engine


Torque driver

- Driver for fastening torque wrench


Submerged full stop drill Surgical kit - I

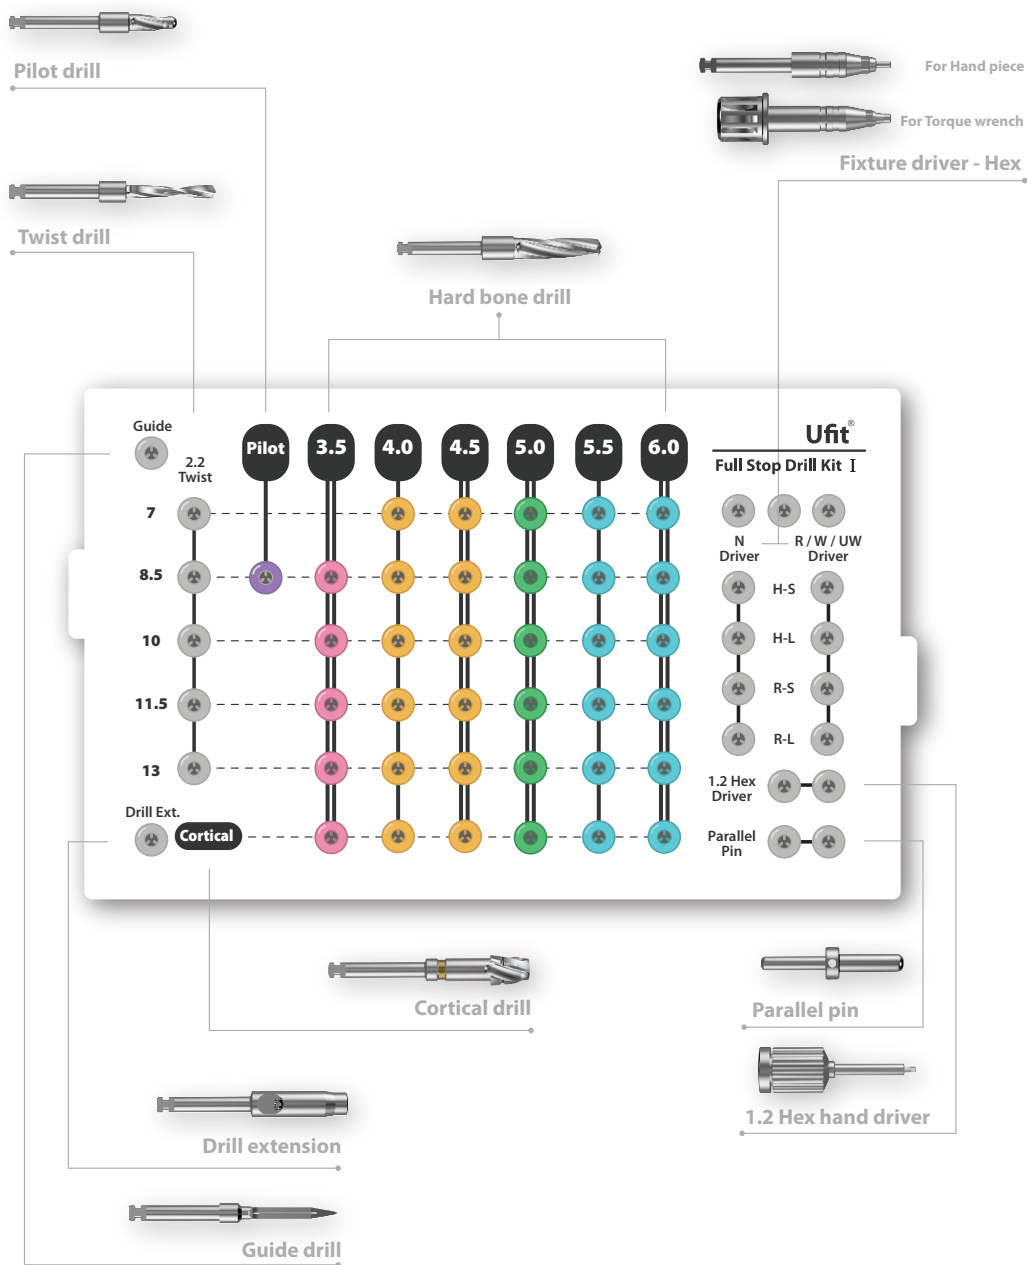


Submerged full stop drill Surgical kit - II

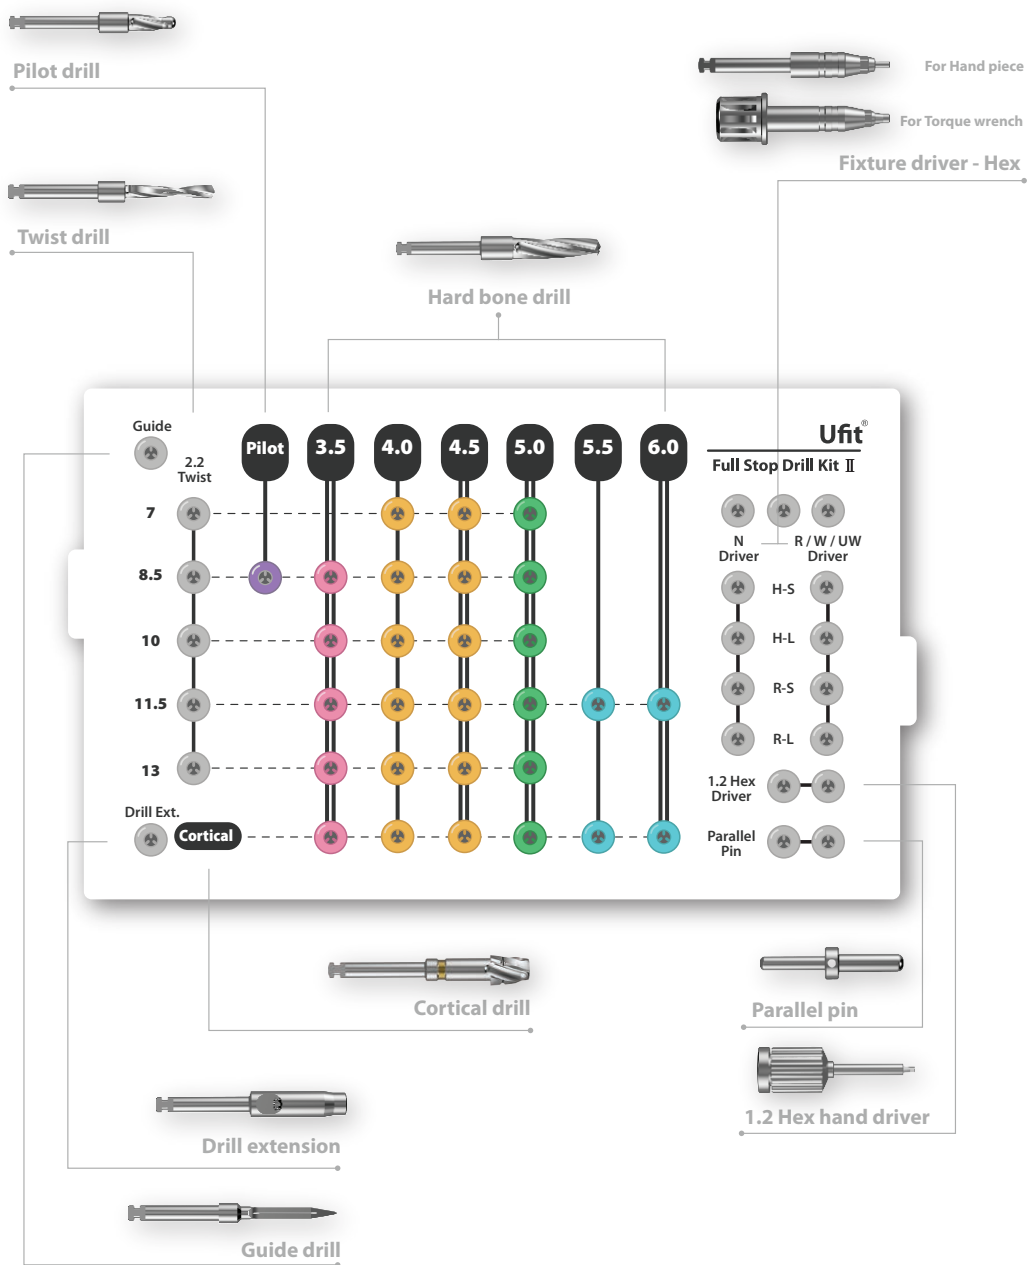

Submerged full stop drill Surgical kit - III

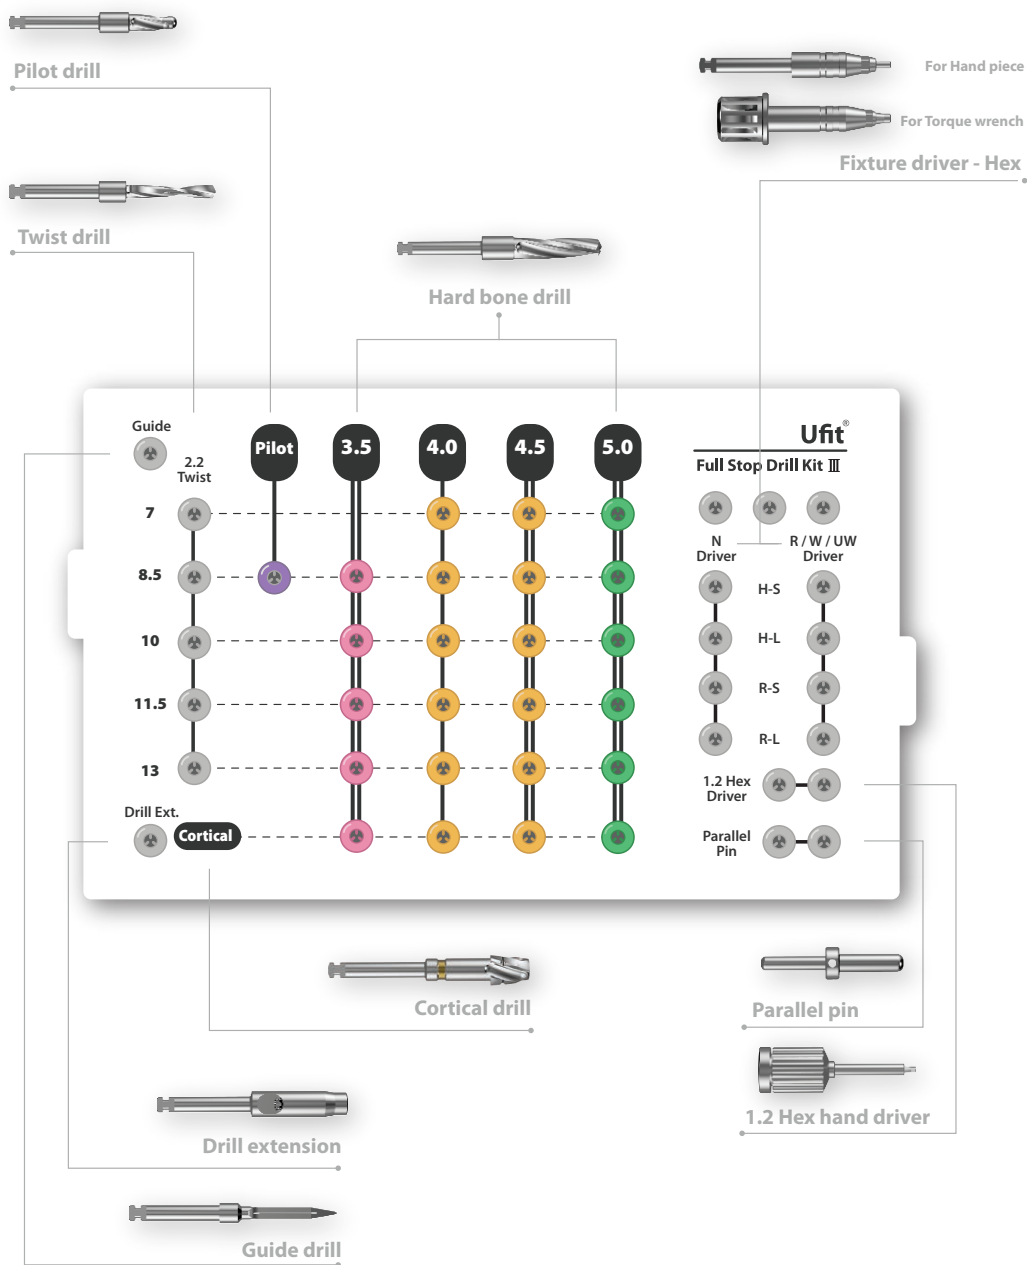




Twist drill

	<i>Diameter</i>	<i>Length</i>
TDR 22075	2.2	7.5
TDR 22085	2.2	8.5
TDR 2210	2.2	10
TDR 22115	2.2	11.5
TDR 2213	2.2	13
TDR 2215	2.2	15

- Initial hole is formed at the marked region by the guide drill
- Caution is used to the adjacent space's depth and parallel



Pilot drill

	<i>D1</i>	<i>D2</i>
PDR 2230	2.2	3.0


- After the initial drilling the Ø2.2 entry way is expanded to Ø3.0 for the tubal drill entry of both the tapered drill and straight drill



Cortical drill

	<i>D2</i>
ICD 35	3.5
ICD 40	4.0
ICD 45	4.5
ICD 50	5.0
ICD 55	5.5
ICD 60	6.0

- Used to prevent the fixture's neck region to be caught in the cortical bone
- composed of the equivalent dimension of the neck-size of the fixture to be inserted.



Hard Bone drill


	<i>D1</i>	<i>D2</i>	<i>Length</i>
<i>IPD 35075</i>	2.6	3.3	7.5
<i>IPD 35085</i>	2.6	3.3	8.5
<i>IPD 3510</i>	2.6	3.3	10
<i>IPD 35115</i>	2.6	3.3	11.5
<i>IPD 3513</i>	2.6	3.3	13
<i>IPD 3515</i>	2.6	3.3	15
<i>IPD 40075</i>	3.1	3.8	7.5
<i>IPD 40085</i>	3.1	3.8	8.5
<i>IPD 4010</i>	3.1	3.8	10
<i>IPD 40115</i>	3.1	3.8	11.5
<i>IPD 4013</i>	3.1	3.8	13
<i>IPD 4015</i>	3.1	3.8	15
<i>IPD 45075</i>	3.6	4.3	7.5
<i>IPD 45085</i>	3.6	4.3	8.5
<i>IPD 4510</i>	3.6	4.3	10
<i>IPD 45115</i>	3.6	4.3	11.5
<i>IPD 4513</i>	3.6	4.3	13
<i>IPD 4515</i>	3.6	4.3	15
<i>IPD 50075</i>	4.1	4.8	7.5
<i>IPD 50085</i>	4.1	4.8	8.5
<i>IPD 5010</i>	4.1	4.8	10
<i>IPD 50115</i>	4.1	4.8	11.5
<i>IPD 5013</i>	4.1	4.8	13
<i>IPD 5015</i>	4.1	4.8	15
<i>IPD 55075</i>	4.6	5.3	7.5
<i>IPD 55085</i>	4.6	5.3	8.5
<i>IPD 5510</i>	4.6	5.3	10
<i>IPD 55115</i>	4.6	5.3	11.5
<i>IPD 5513</i>	4.6	5.3	13
<i>IPD 5515</i>	4.6	5.3	15
<i>IPD 60075</i>	5.1	5.8	7.5
<i>IPD 60085</i>	5.1	5.8	8.5
<i>IPD 6010</i>	5.1	5.8	10
<i>IPD 60115</i>	5.1	5.8	11.5
<i>IPD 6013</i>	5.1	5.8	13
<i>IPD 6015</i>	5.1	5.8	15

- Used to expand the dimension of the equivalent body size of the fixture to be inserted into the Ø2.2 hole that is formed by twist drilling.


- To minimize bone resistance in order to prevent bone crack, necrosis and others, drills are used in stages starting with the smallest diameter.

- Fixture's own body shape is almost equivalent to the body shape

Submerged full stop drill kit drilling sequence

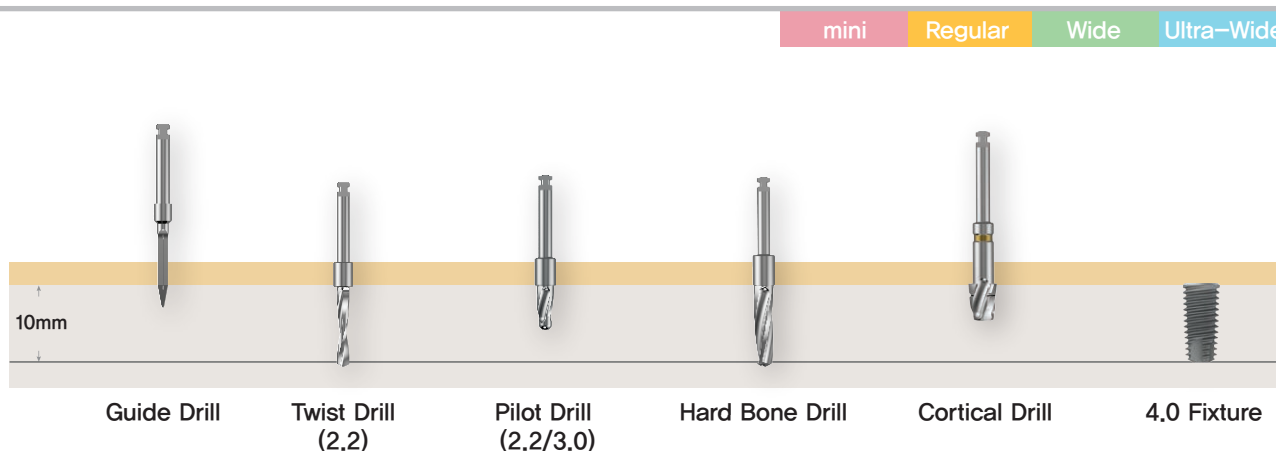


3.5 Fixture

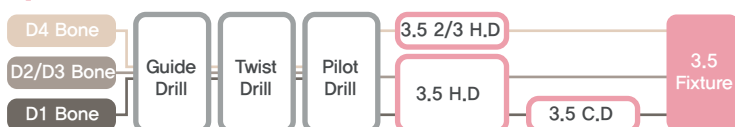


H.D : Hard Bone Drill [D – 0.2]
C.D : Cortical Drill [D – 0.0]


4.0 Fixture

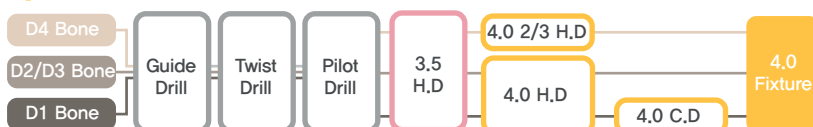

4.5 Fixture

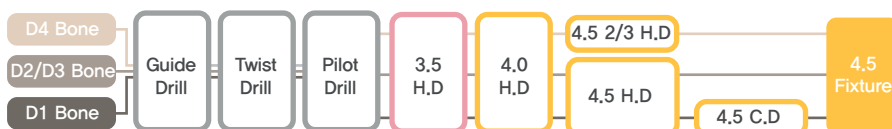

5.0 Fixture

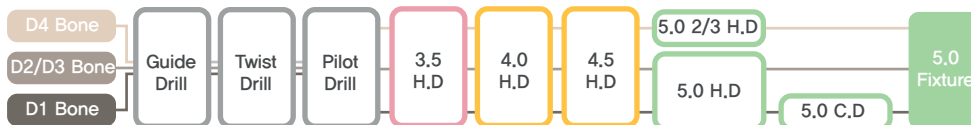


5.5 Fixture




6.0 Fixture




Internal full stop drill Surgical kit - I

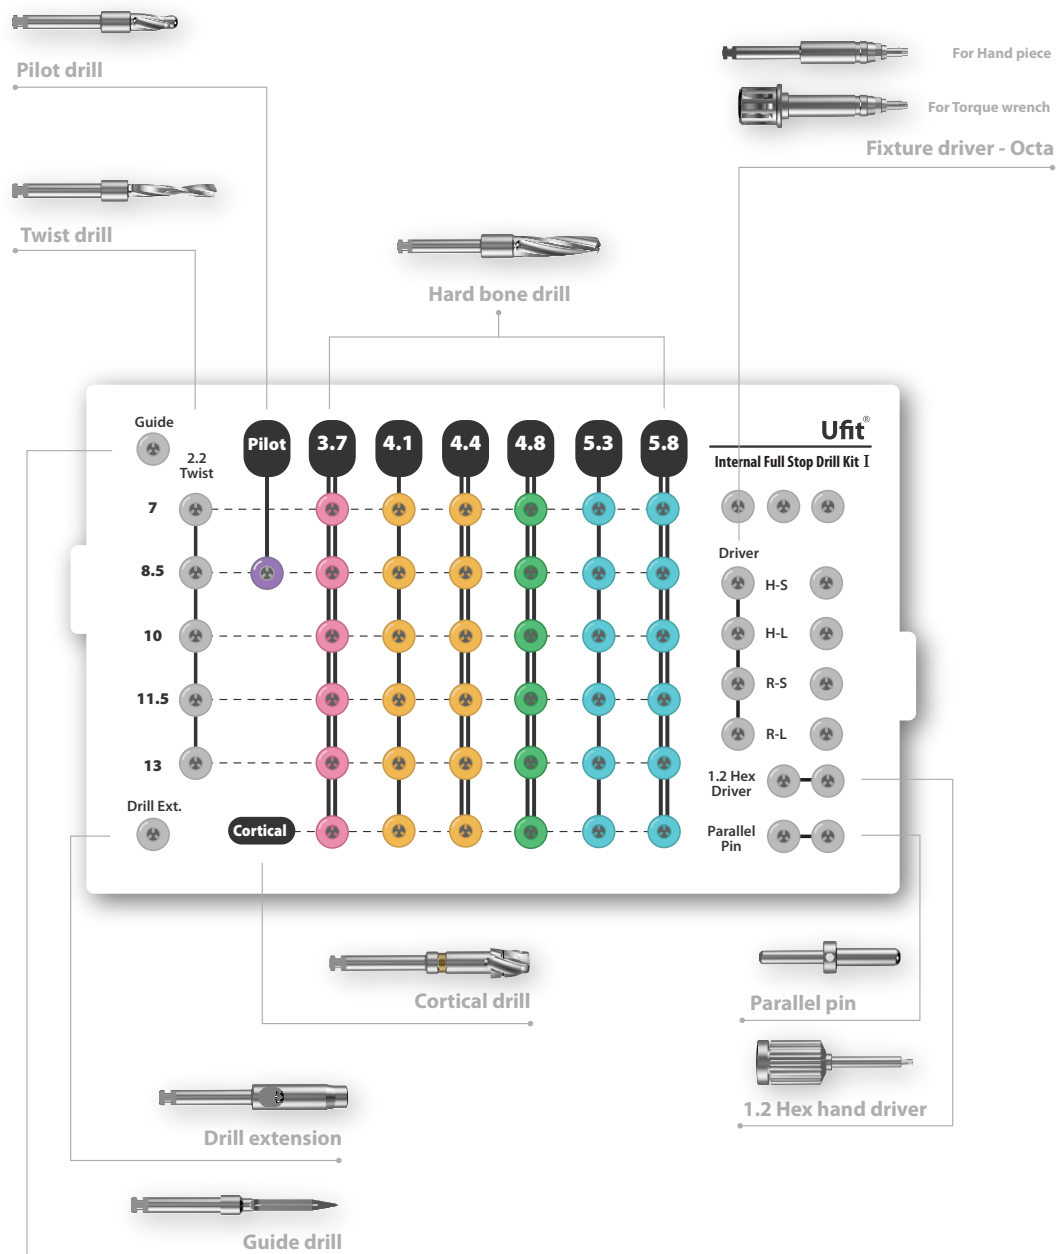


Internal full stop drill Surgical kit - II

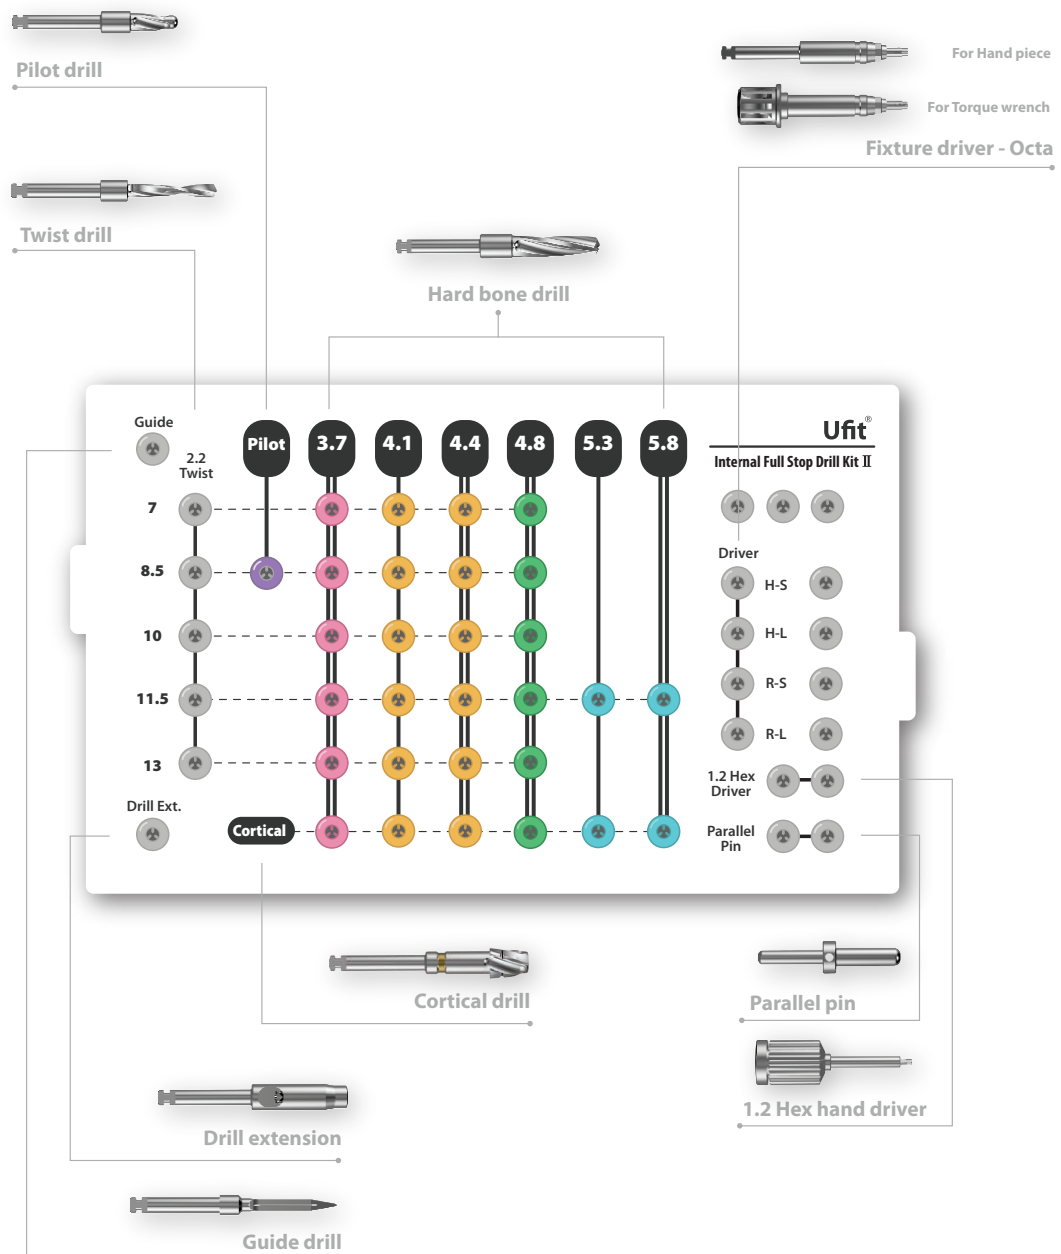

Internal full stop drill Surgical kit - III

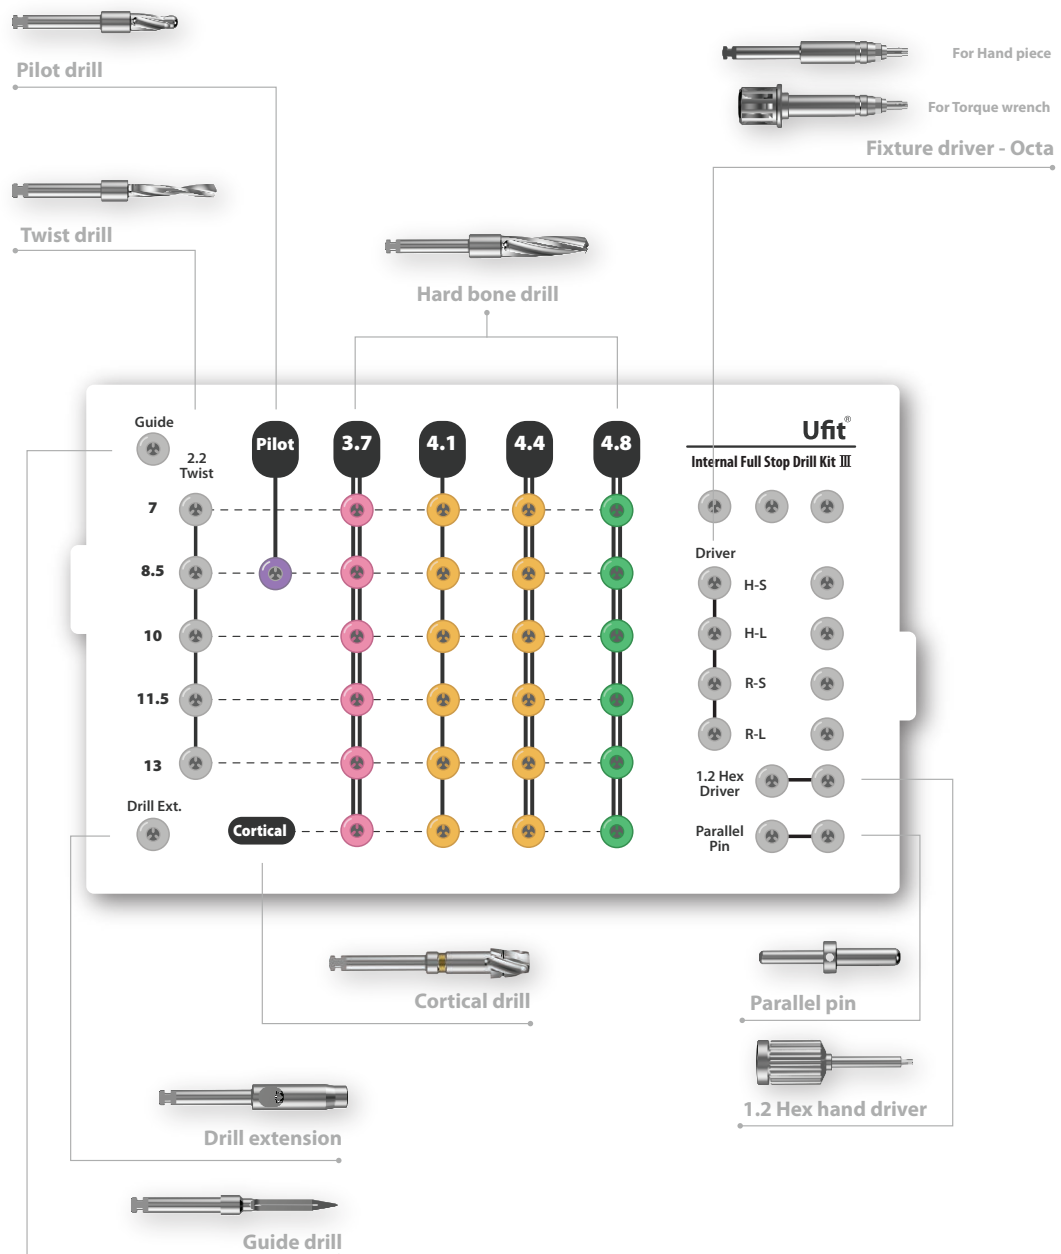




Twist drill

	<i>Diameter</i>	<i>Length</i>
TDR 22075	2.2	7.5
TDR 22085	2.2	8.5
TDR 2210	2.2	10
TDR 22115	2.2	11.5
TDR 2213	2.2	13
TDR 2215	2.2	15

- Initial hole is formed at the marked region by the guide drill
- Caution is used to the adjacent space's depth and parallel



Pilot drill

	<i>D1</i>	<i>D2</i>
PDR 2230	2.2	3.0


- After the initial drilling the Ø2.2 entry way is expanded to Ø3.0 for the tubal drill entry of both the tapered drill and straight drill



Cortical drill

	<i>D2</i>
ICD 37	3.9
ICD 41	4.1
ICD 44	4.4
ICD 48	4.8
ICD 53	5.3
ICD 58	5.8

- Used to prevent the fixture's neck region to be caught in the cortical bone
- composed of the equivalent dimension of the neck-size of the fixture to be inserted.



Hard Bone drill

	<i>D1</i>	<i>D2</i>	<i>Length</i>
<i>IPD 37075</i>	2.8	3.5	7.5
<i>IPD 37085</i>	2.8	3.5	8.5
<i>IPD 3710</i>	2.8	3.5	10
<i>IPD 37115</i>	2.8	3.5	11.5
<i>IPD 3713</i>	2.8	3.5	13
<i>IPD 3715</i>	2.8	3.5	15
<i>IPD 41075</i>	3.2	3.9	7.5
<i>IPD 41085</i>	3.2	3.9	8.5
<i>IPD 4110</i>	3.2	3.9	10
<i>IPD 41115</i>	3.2	3.9	11.5
<i>IPD 4113</i>	3.2	3.9	13
<i>IPD 4115</i>	3.2	3.9	15
<i>IPD 44075</i>	3.5	4.2	7.5
<i>IPD 44085</i>	3.5	4.2	8.5
<i>IPD 4410</i>	3.5	4.2	10
<i>IPD 44115</i>	3.5	4.2	11.5
<i>IPD 4413</i>	3.5	4.2	13
<i>IPD 4415</i>	3.5	4.2	15
<i>IPD 48075</i>	3.9	4.6	7.5
<i>IPD 48085</i>	3.9	4.6	8.5
<i>IPD 4810</i>	3.9	4.6	10
<i>IPD 48115</i>	3.9	4.6	11.5
<i>IPD 4813</i>	3.9	4.6	13
<i>IPD 4815</i>	3.9	4.6	15
<i>IPD 53075</i>	4.4	5.1	7.5
<i>IPD 53085</i>	4.4	5.1	8.5
<i>IPD 5310</i>	4.4	5.1	10
<i>IPD 53115</i>	4.4	5.1	11.5
<i>IPD 5313</i>	4.4	5.1	13
<i>IPD 5315</i>	4.4	5.1	15
<i>IPD 58075</i>	4.9	5.6	7.5
<i>IPD 58085</i>	4.9	5.6	8.5
<i>IPD 5810</i>	4.9	5.6	10
<i>IPD 58115</i>	4.9	5.6	11.5
<i>IPD 5813</i>	4.9	5.6	13
<i>IPD 5815</i>	4.9	5.6	15


- Used to expand the dimension of the equivalent body size of the fixture to be inserted into the Ø2.2 hole that is formed by twist drilling.

- To minimize bone resistance in order to prevent bone crack, necrosis and others, drills are used in stages starting with the smallest diameter.


- Fixture's own body shape is almost equivalent to the body shape

Internal full stop drill kit drilling sequence

Narrow Regular Wide Ultra-Wide

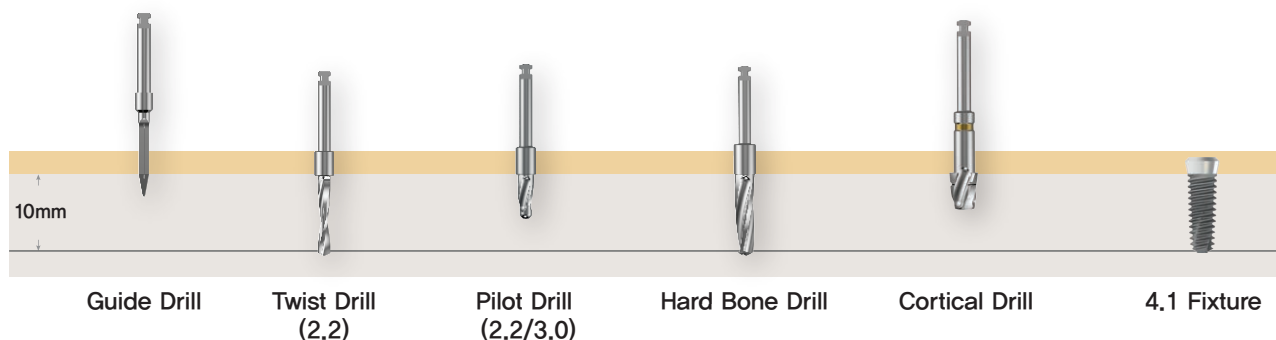


3.7 Fixture

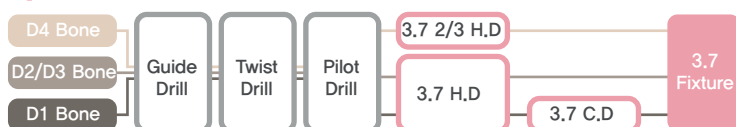


H.D : Hard Bone Drill [D – 0.2]
C.D : Cortical Drill [D – 0.0]


4.1 Fixture

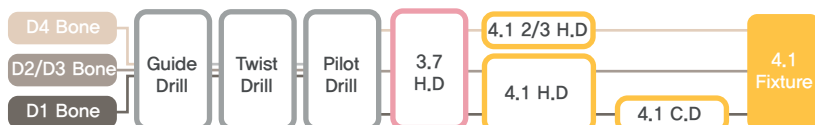

4.4 Fixture

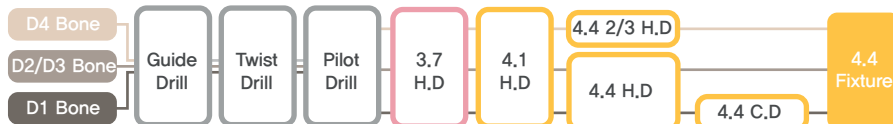

4.8 Fixture

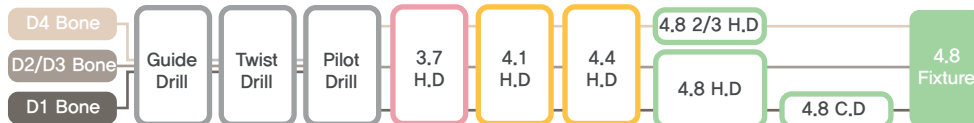

5.3 Fixture



5.8 Fixture



Ufit implant Certificates.

FDA



ISO 13485



ISO 9001




CE 0120 Certificate




GMP Certificate



Domestic Patent

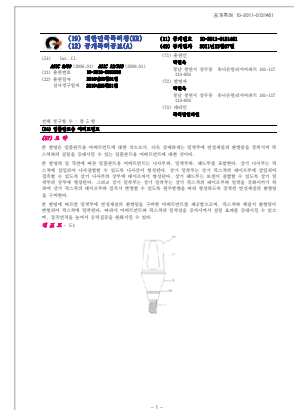

Domestic Patent

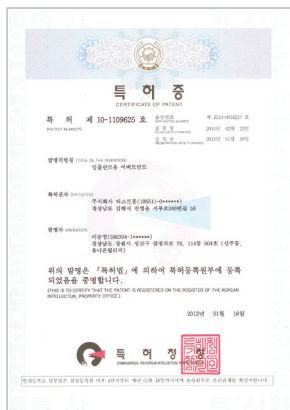

Japan Patent



China Patent



Ufit[®] dental implant

January. 04. 2018

T.Strong INC.

Tel. +82 55 342 1771 Fax. +82 55 342 1775

56, Seobu-ro 346beon-gil, Jinyeong-eup, Gimhae-si,
Gyeongsangnam-do, 50870, Rep. of KOREA

Copyright © 2018 by T.Strong INC. All Right Reserved.



CE
0120



Ufit[®]

www.ufitimplant.com

T.STRONG INC.

Tel. +82 55 342 1771 Fax. +82 55 342 1775

56, Seobu-ro 346beon-gil, Jinyeong-eup, Gimhae-si,
Gyeongsangnam-do, 50870, Rep. of KOREA

